

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/05/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:24
INTERNAL STANDARD	VERIFIED	00:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:26
BLANK TEST	0.00	00:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:27
BLANK TEST	0.00	00:28

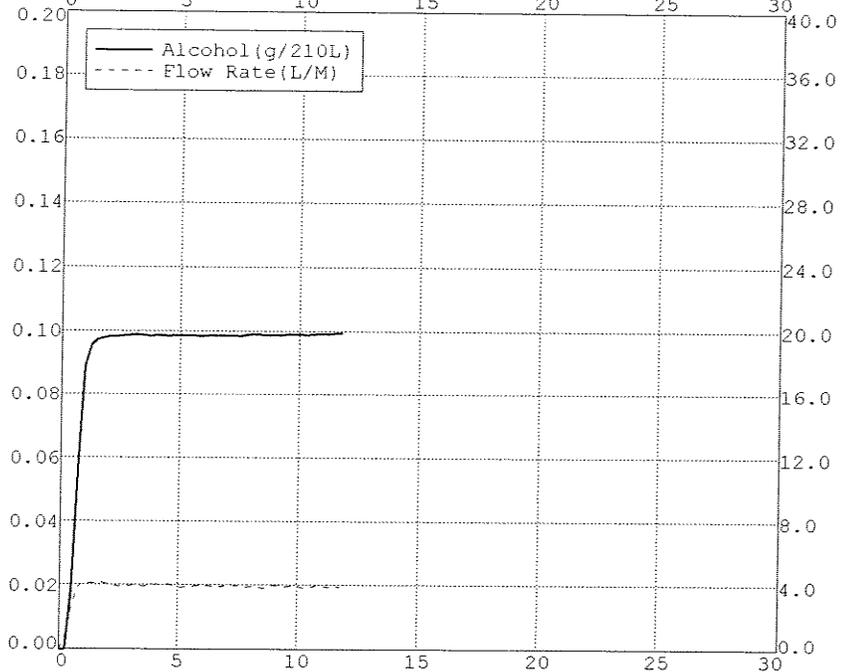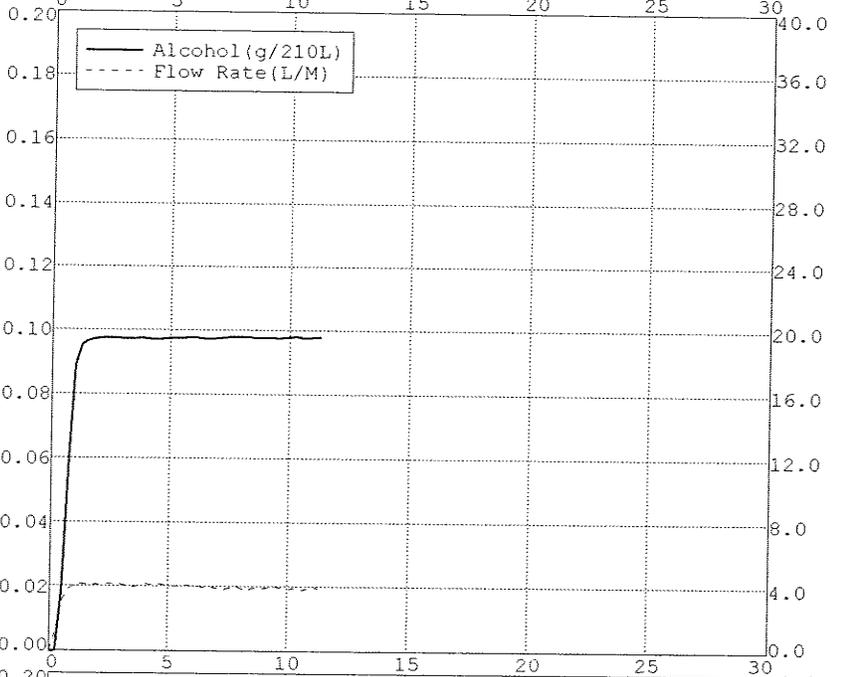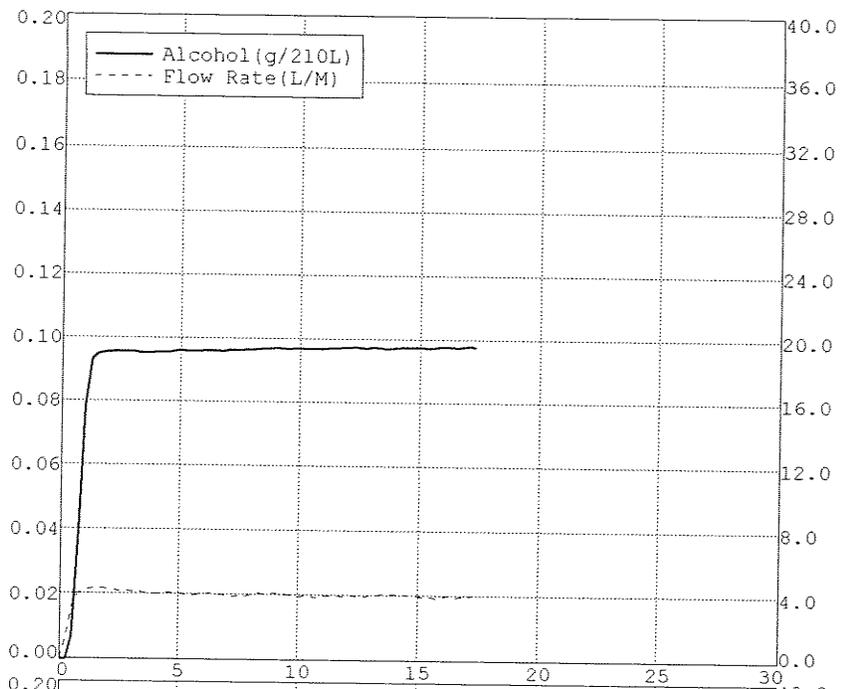

SGS R.J. Bartlett
WCSO #162 12-5-16