

SUPERVISOR TEST




-----  
 WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208  
 -----

Date: 12/13/2016

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:37
INTERNAL STANDARD	VERIFIED	01:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:38
BLANK TEST	0.00	01:39
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:39
BLANK TEST	0.00	01:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:40
BLANK TEST	0.00	01:41

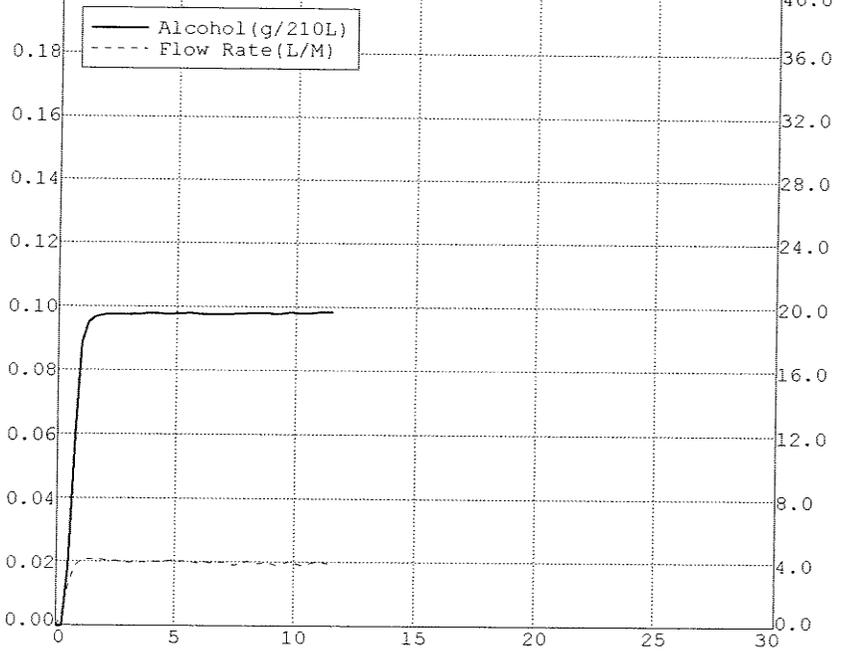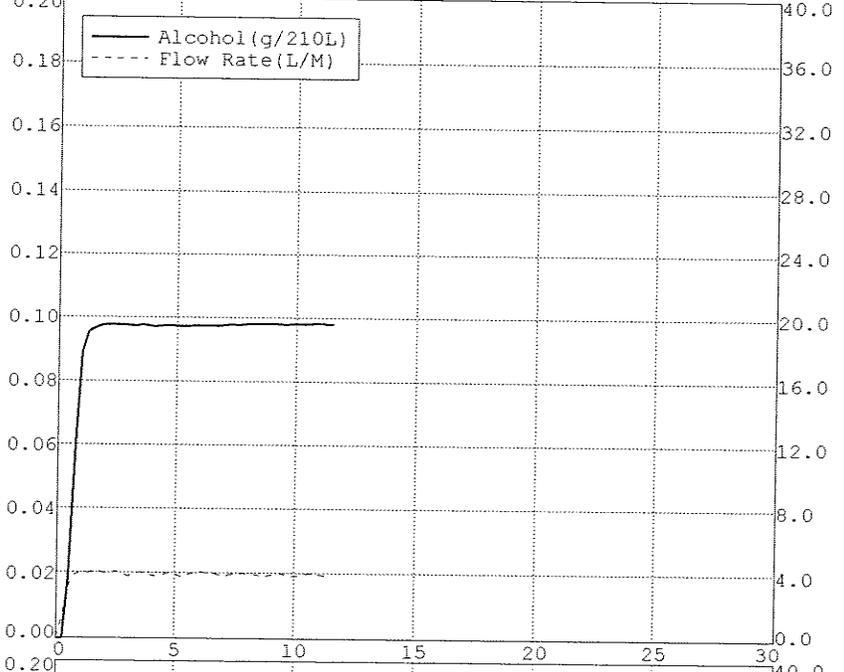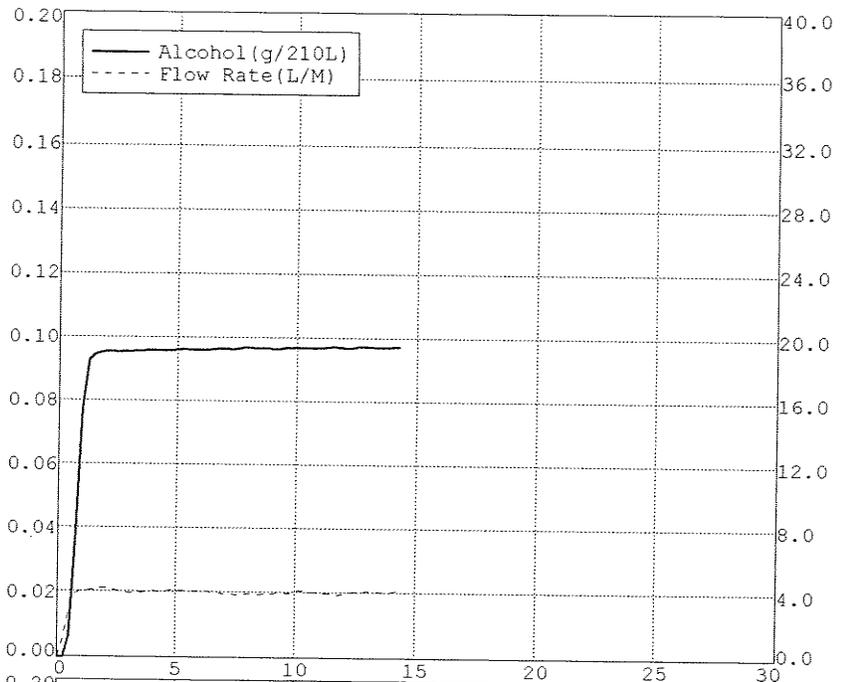

SCR RJB Bartlett WISO #162  
 12-13-16