

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/27/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:02
INTERNAL STANDARD	VERIFIED	00:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:03
BLANK TEST	0.00	00:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:04
BLANK TEST	0.00	00:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:05
BLANK TEST	0.00	00:06

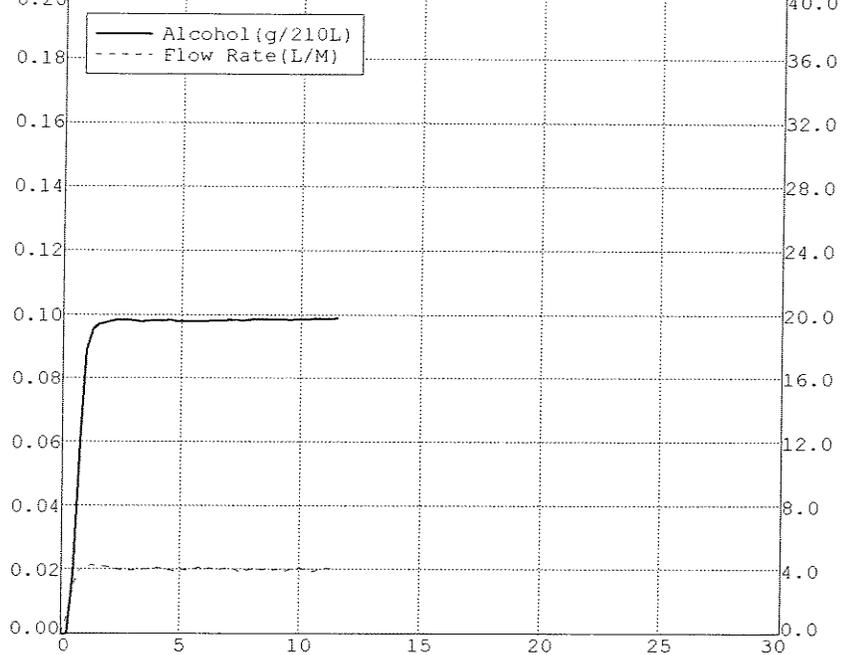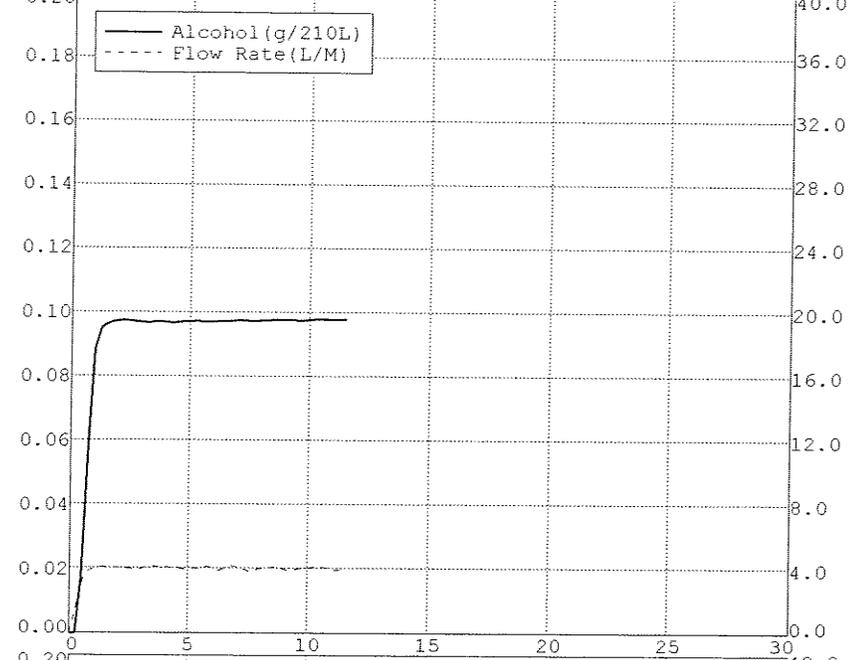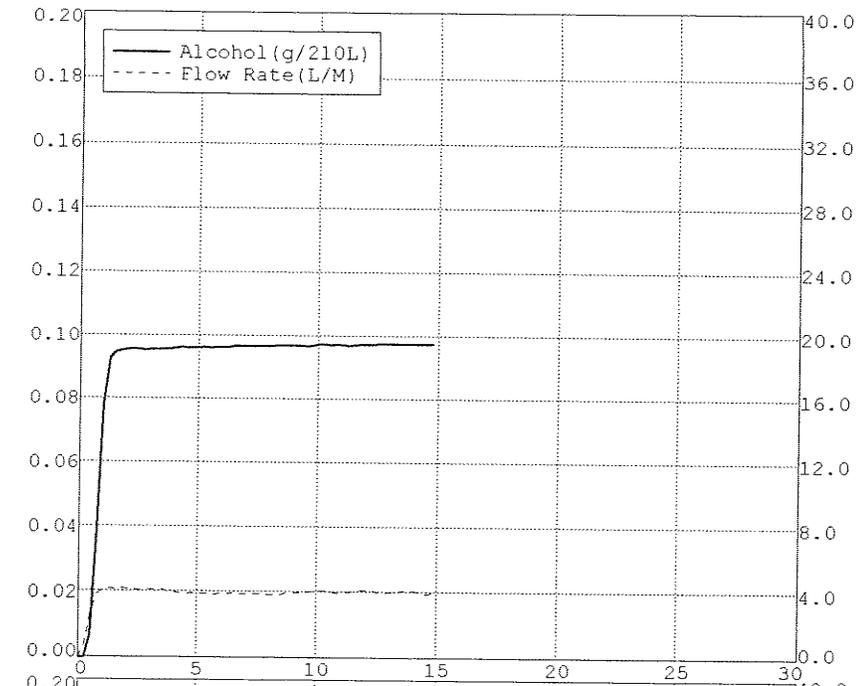

SGS RJA Bartlett WCSO #162
12-27-16