

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/12/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15210

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:01
INTERNAL STANDARD	VERIFIED	00:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:02
BLANK TEST	0.00	00:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:03
BLANK TEST	0.00	00:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:05
BLANK TEST	0.00	00:06

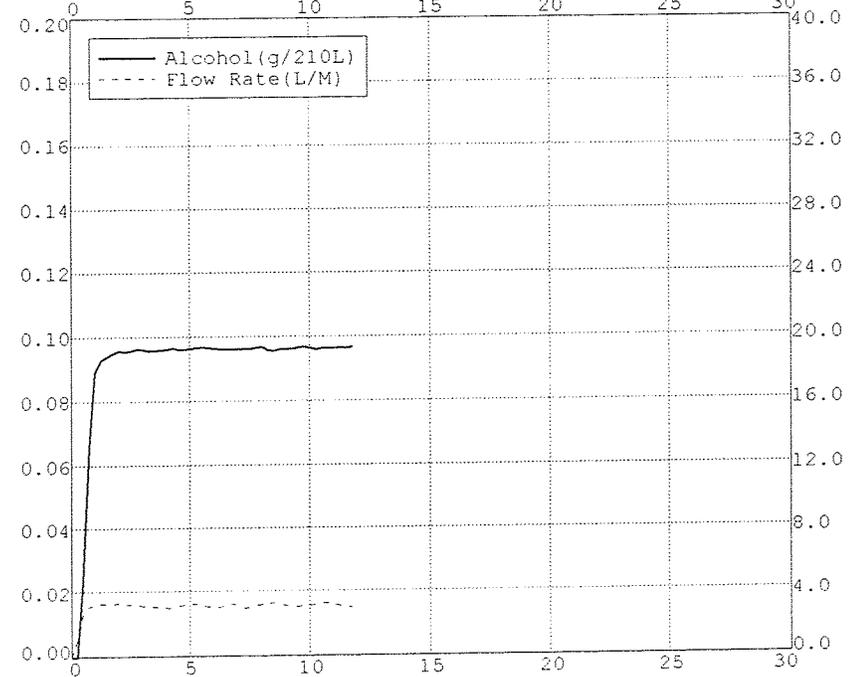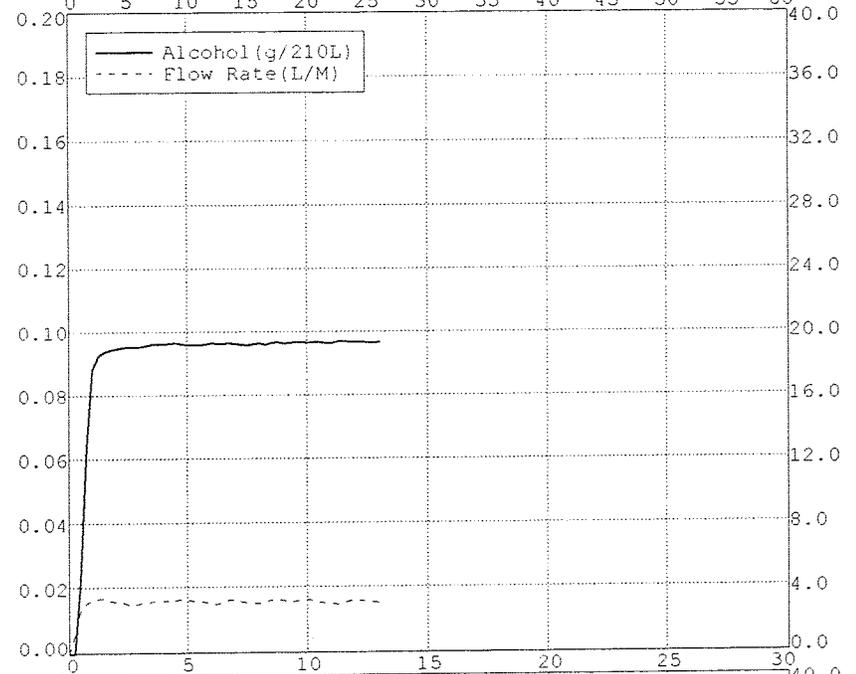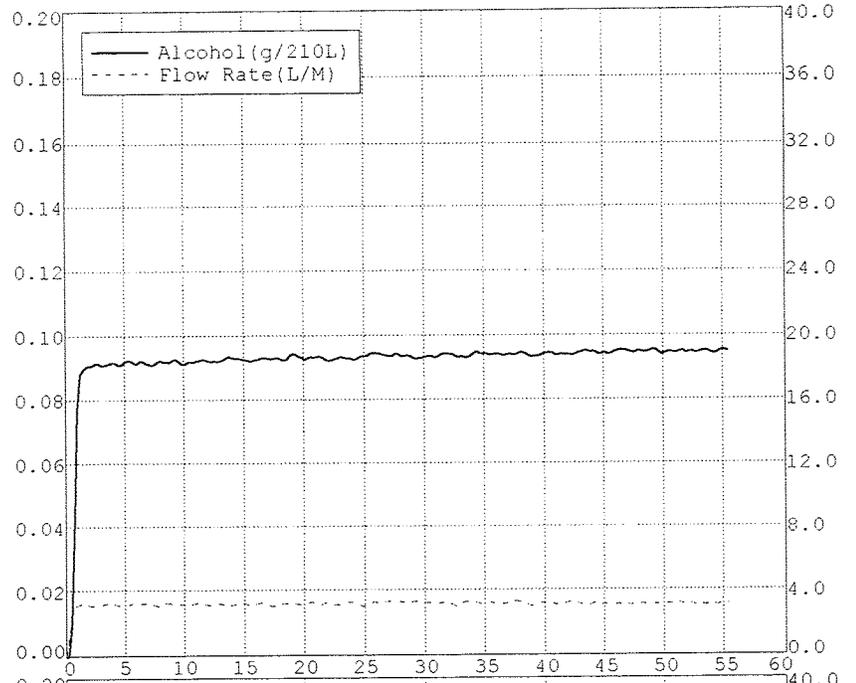

Sgt Ralph Bartlett

WCSO #162

01-12-16