

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/09/2016

OPERATOR NAME:
KENNETH W SMITH
Permit #: 35604
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:05
INTERNAL STANDARD	VERIFIED	23:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:06
BLANK TEST	0.00	23:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:07
BLANK TEST	0.00	23:08
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:08
BLANK TEST	0.00	23:09

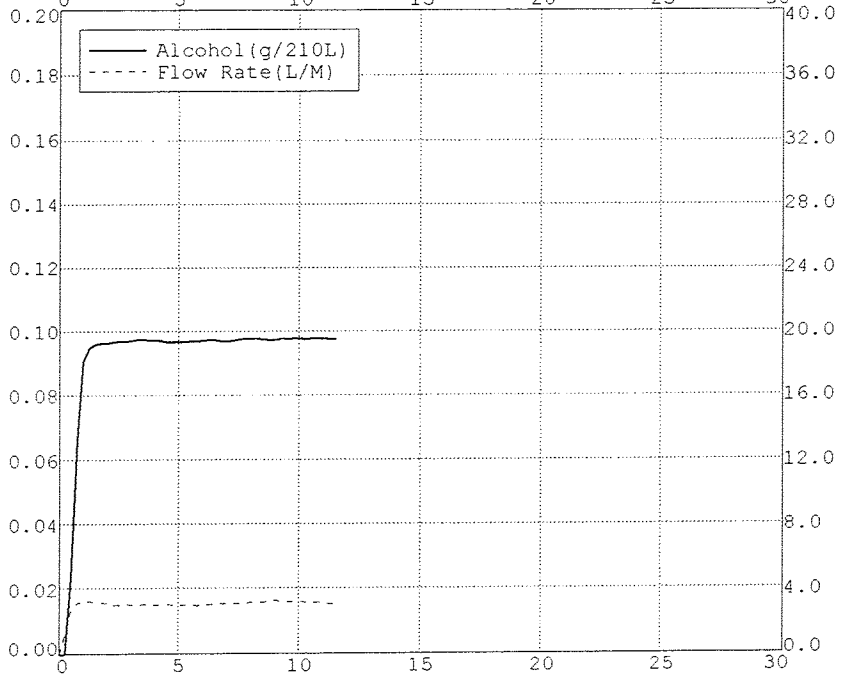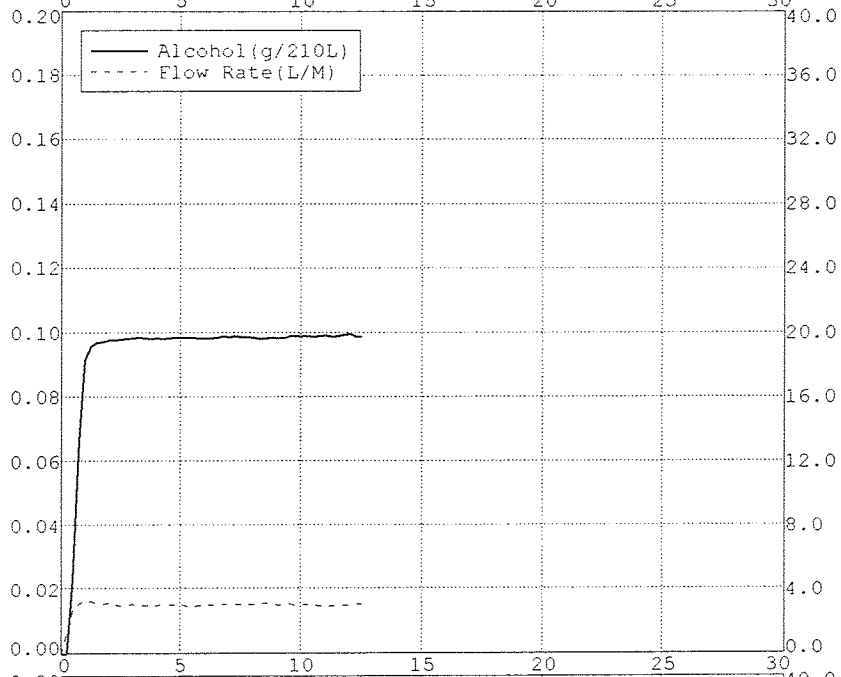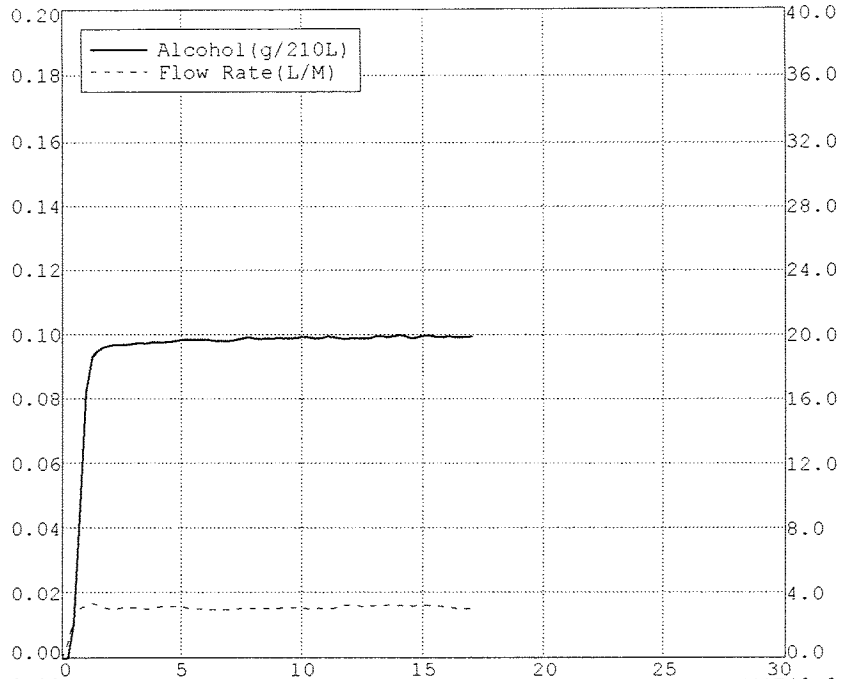

Handwritten signature: Kenneth W. Smith
301
02/09/16

Queensbury