

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/17/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:50
INTERNAL STANDARD	VERIFIED	13:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:50
BLANK TEST	0.00	13:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:52
BLANK TEST	0.00	13:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:53
BLANK TEST	0.00	13:54

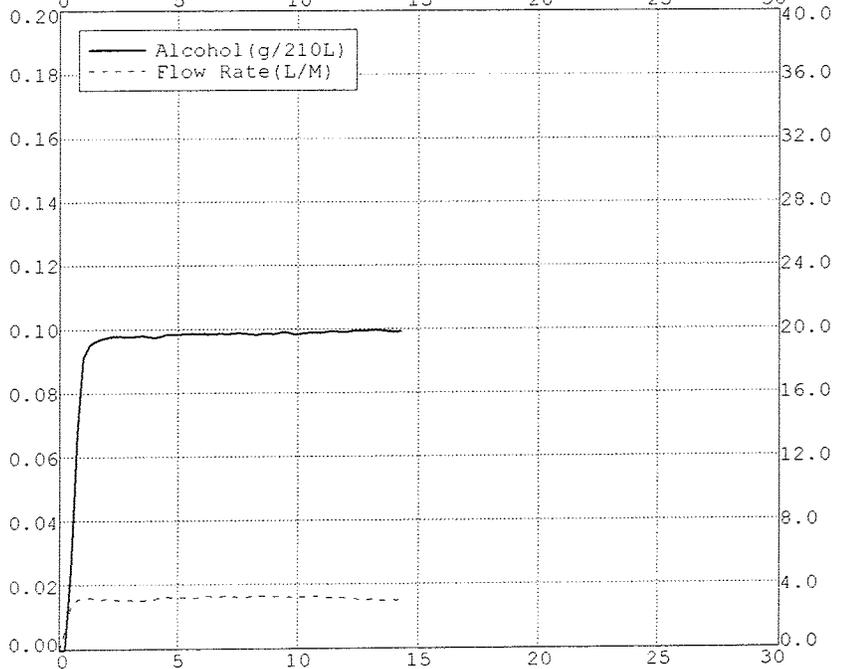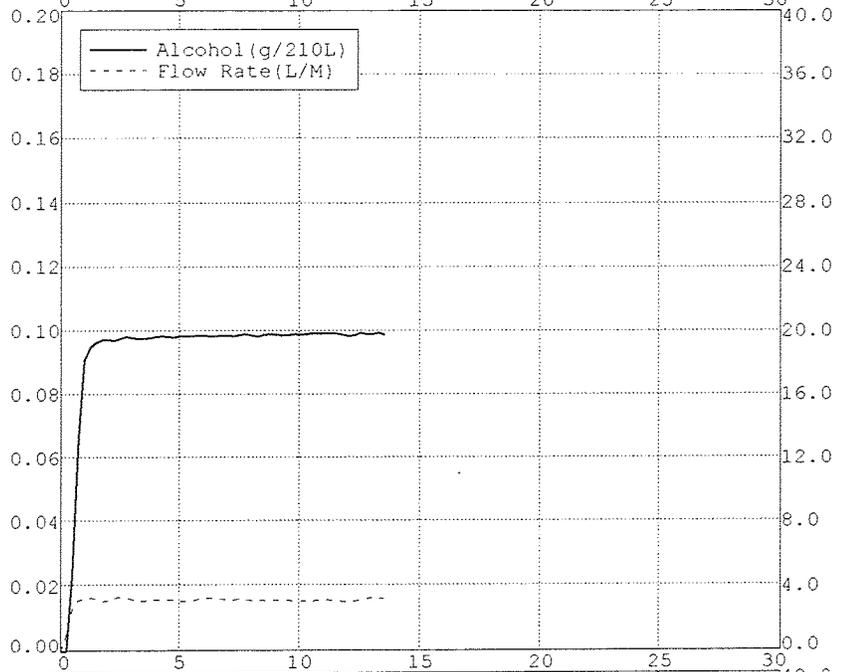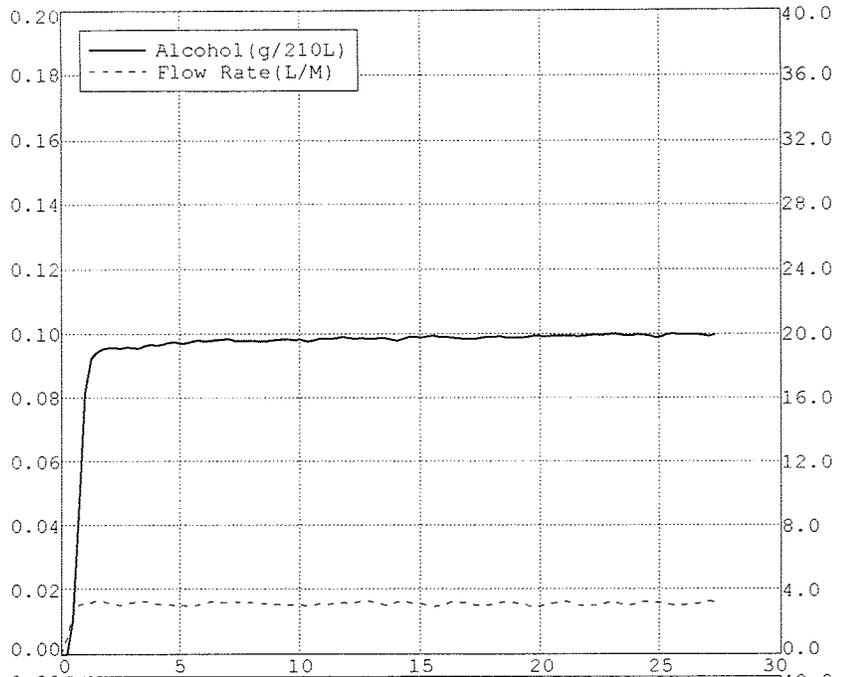

SGS Rpt, ~~Flow~~ WASO #162
02-17-16