

SUPERVISOR TEST



 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 02/22/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:40
INTERNAL STANDARD	VERIFIED	23:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:41
BLANK TEST	0.00	23:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:42
BLANK TEST	0.00	23:43
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:44
BLANK TEST	0.00	23:44

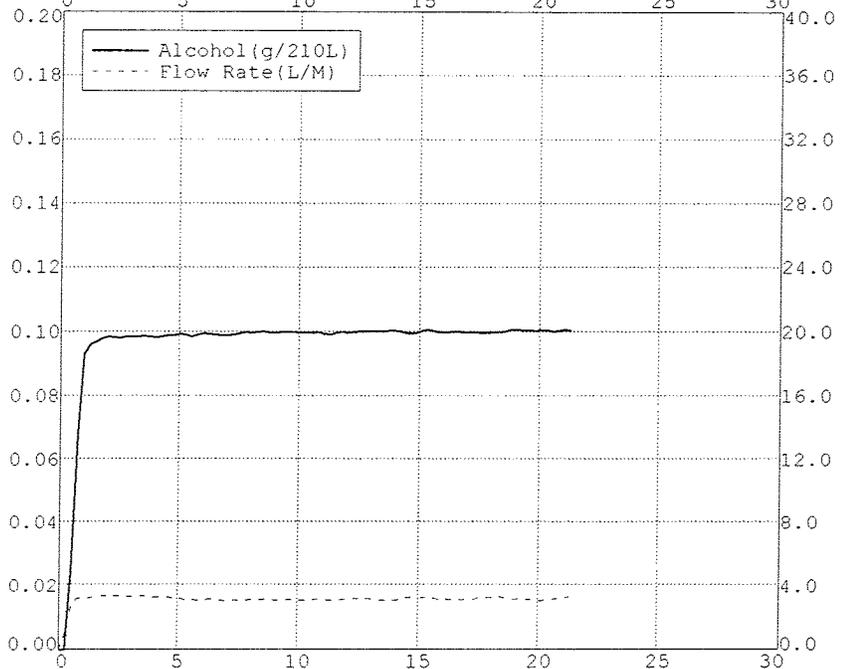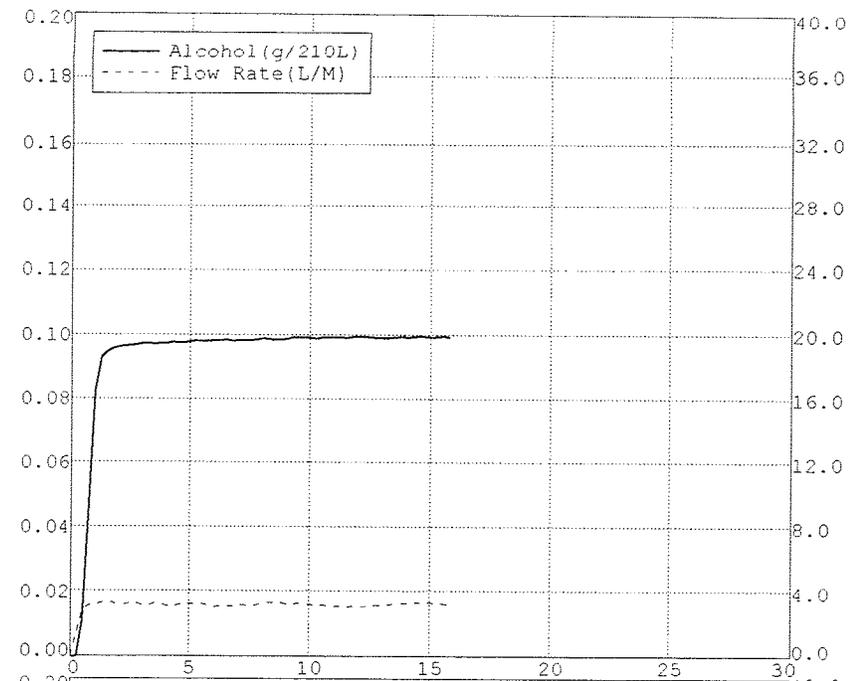

see Reg Borden waso #162
 02-22-16