

SOLUTION CHANGE




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 02/29/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:02
INTERNAL STANDARD	VERIFIED	02:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:02
BLANK TEST	0.00	02:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:03
BLANK TEST	0.00	02:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:05
BLANK TEST	0.00	02:05

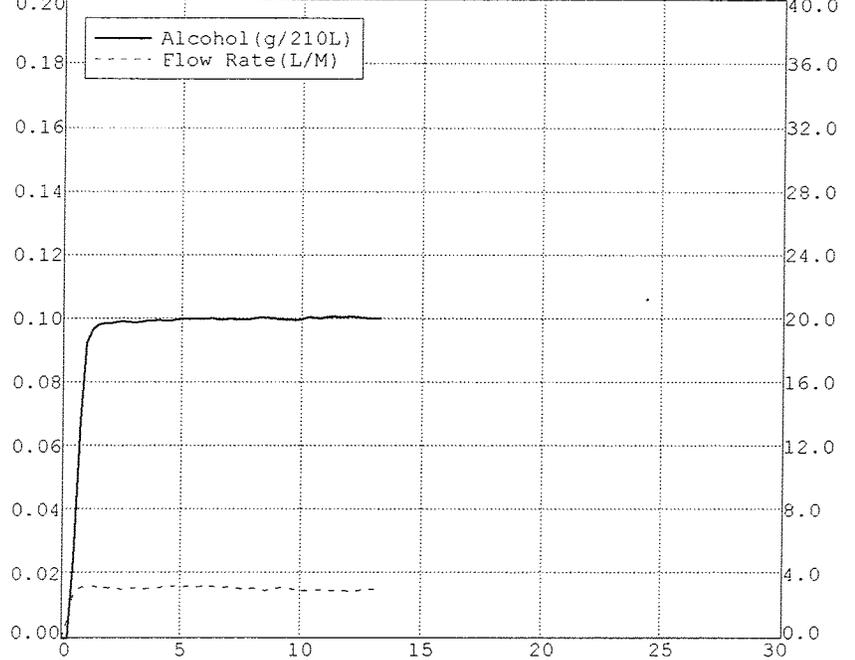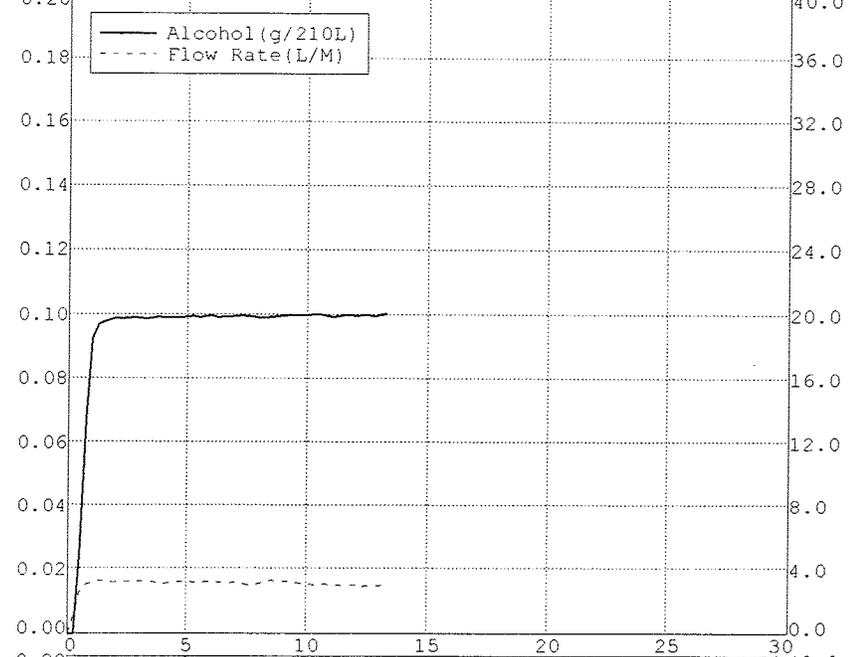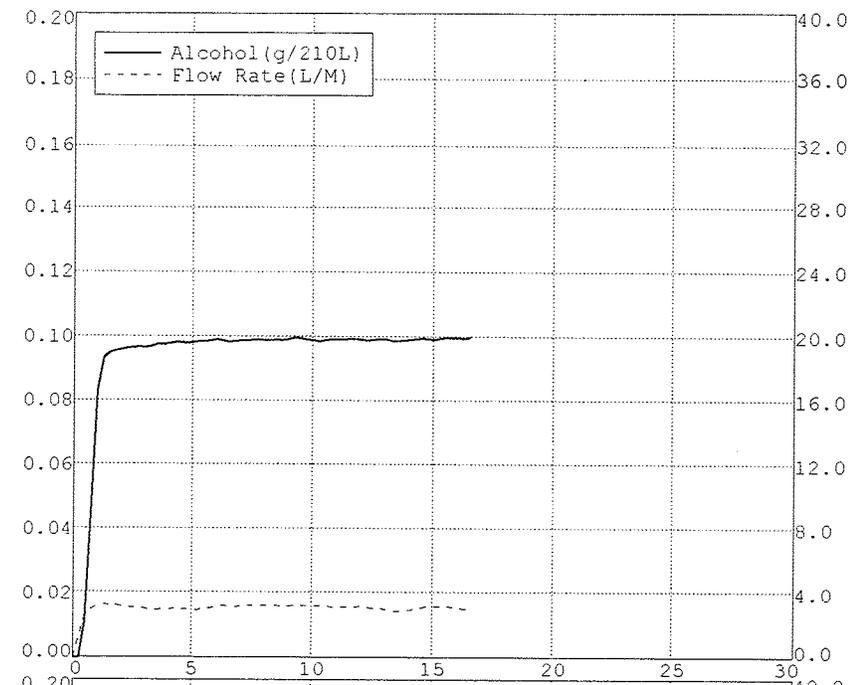

SGS Ref, Bureau W-50 # 162
 02-29-16