

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/08/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:27
INTERNAL STANDARD	VERIFIED	02:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:27
BLANK TEST	0.00	02:28
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:29
BLANK TEST	0.00	02:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:30
BLANK TEST	0.00	02:31

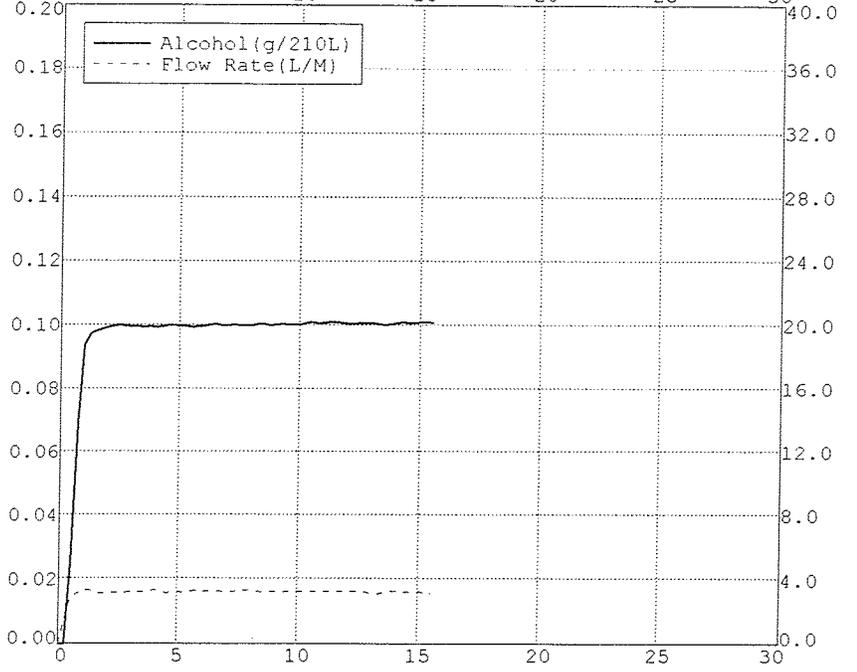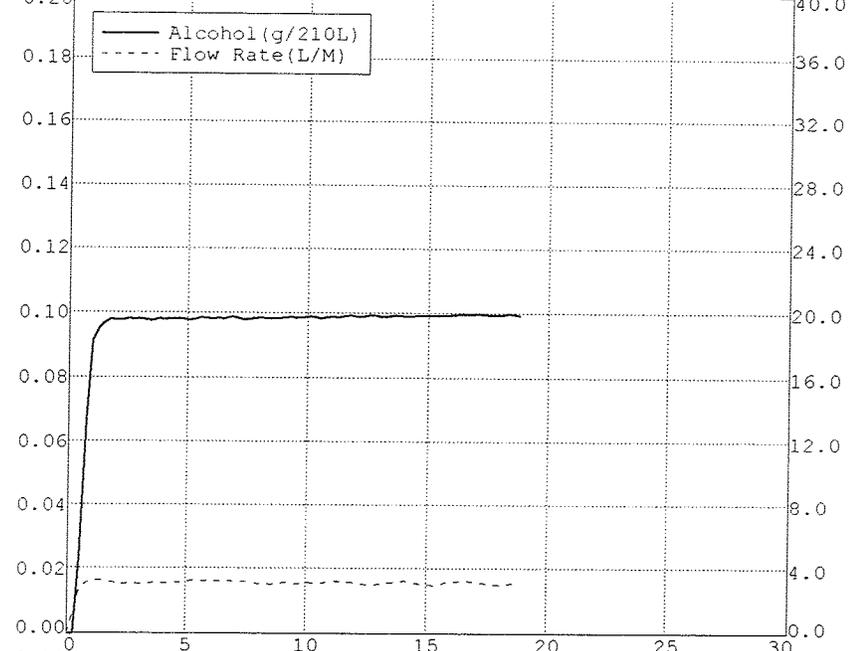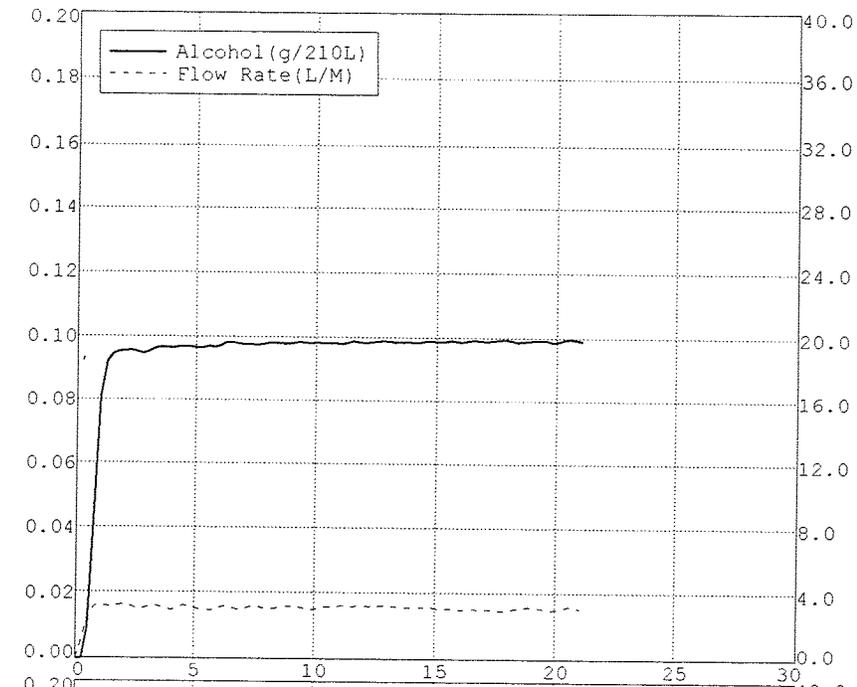

SOS Dept, Bartlett WCSO #162

03-08-16