

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 03/18/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:33
INTERNAL STANDARD	VERIFIED	02:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:33
BLANK TEST	0.00	02:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:35
BLANK TEST	0.00	02:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:36
BLANK TEST	0.00	02:37

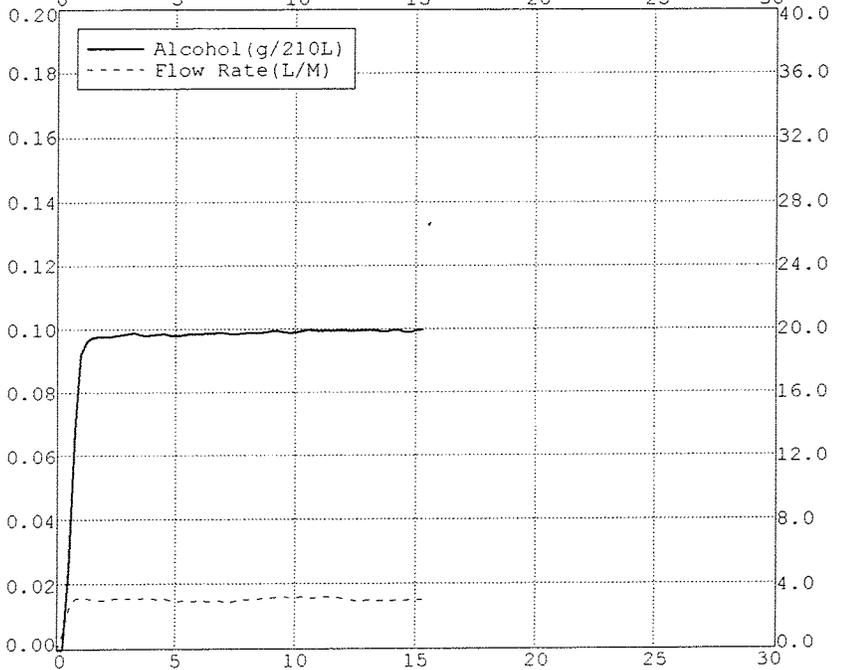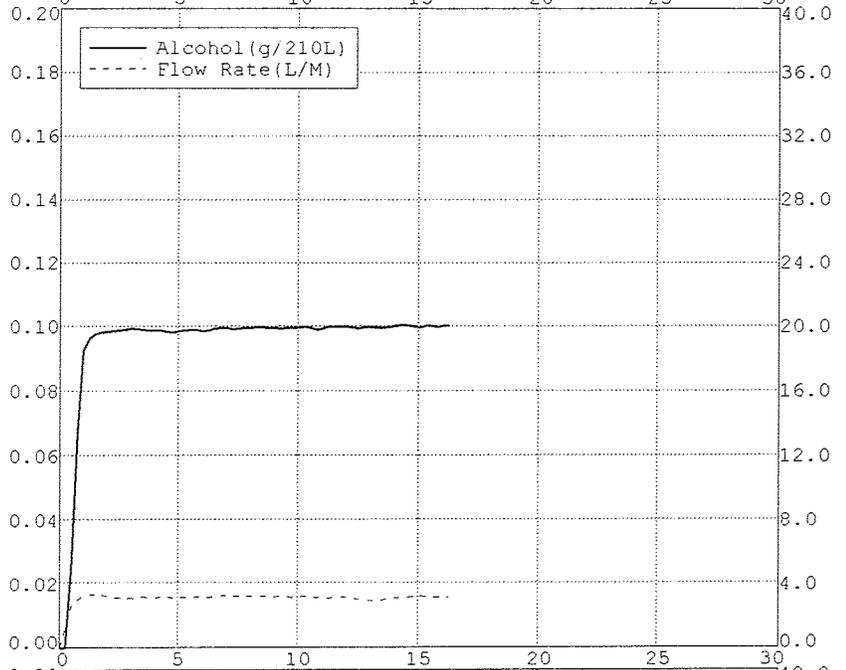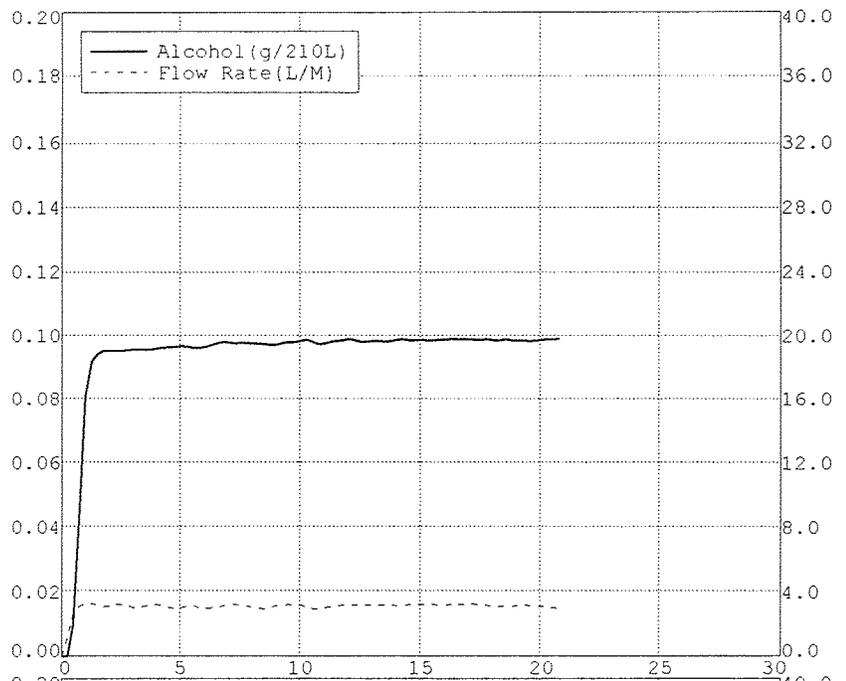

*See Rly Results case #162*

03-18-16