

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 03/28/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:02
INTERNAL STANDARD	VERIFIED	00:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:03
BLANK TEST	0.00	00:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:04
BLANK TEST	0.00	00:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:05
BLANK TEST	0.00	00:06

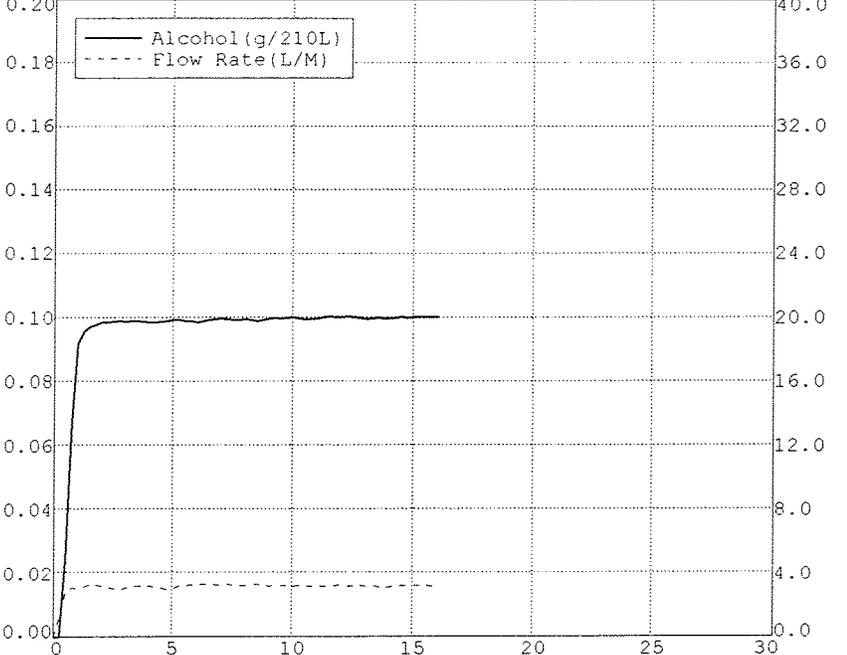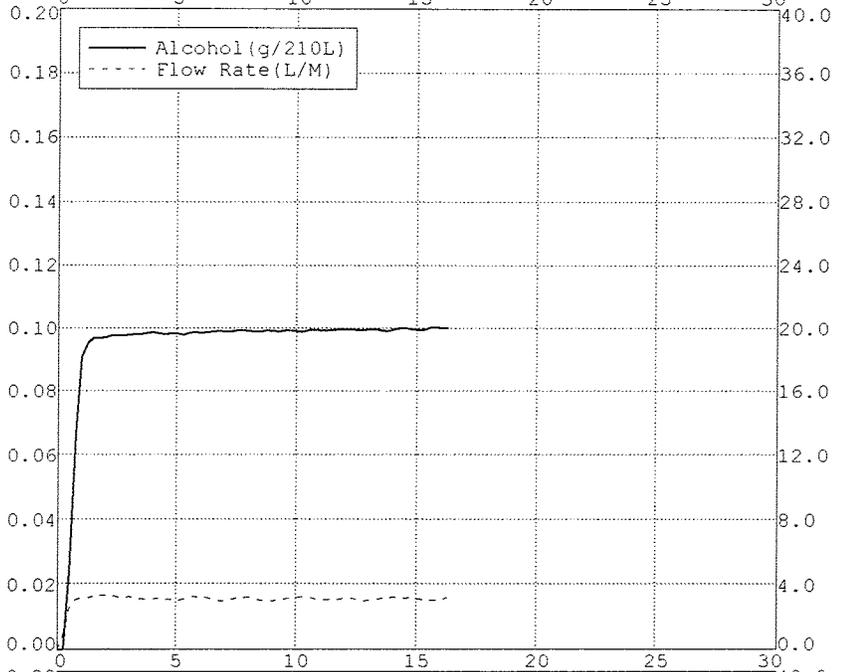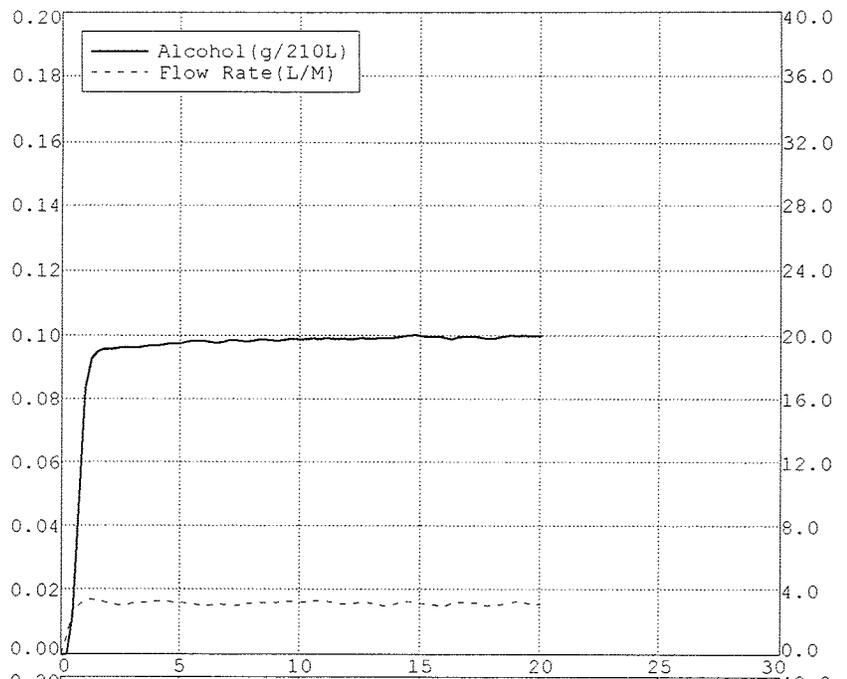

515 Ralph Bartlett
WCSO # 162 03-28-16