

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/03/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16050

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:05
INTERNAL STANDARD	VERIFIED	00:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:05
BLANK TEST	0.00	00:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:07
BLANK TEST	0.00	00:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:08
BLANK TEST	0.00	00:09

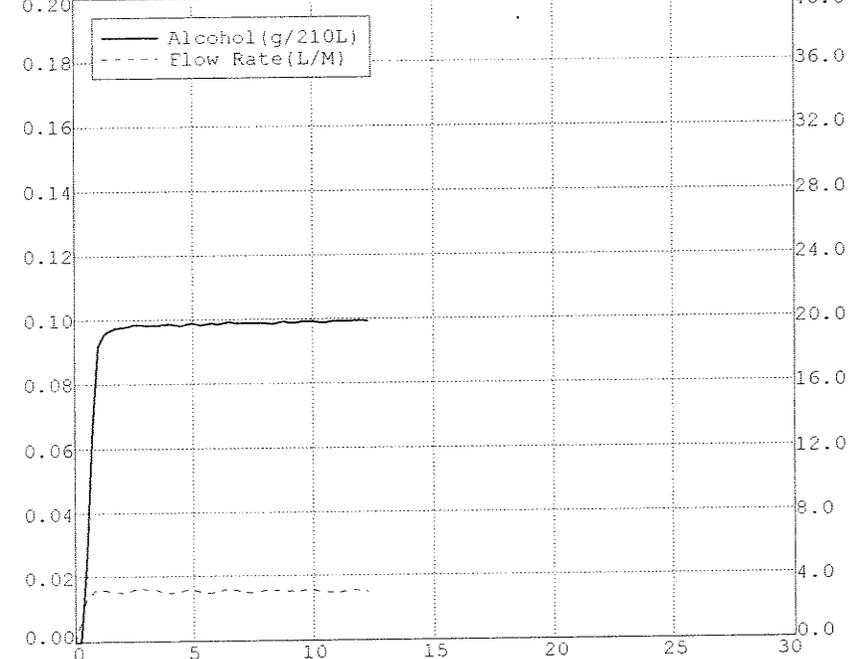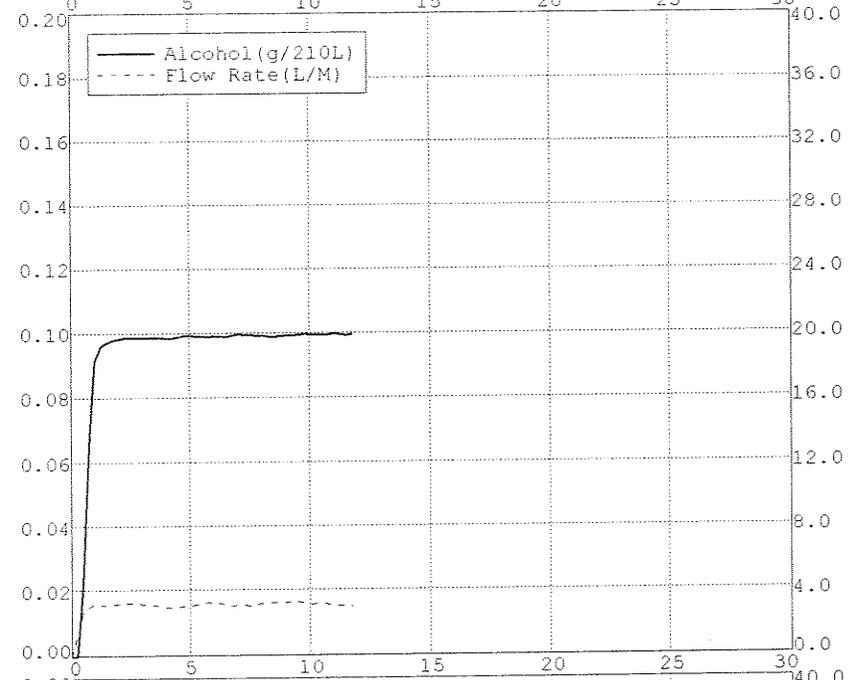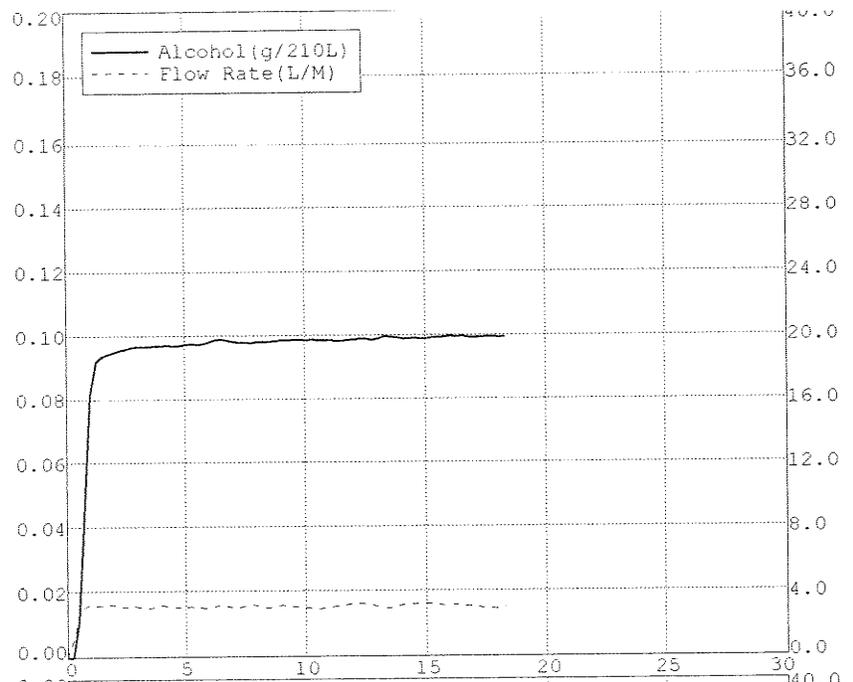

505 Ralph J Bartlett 05-03-16
WC10 #162