

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 05/09/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16050

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:05
INTERNAL STANDARD	VERIFIED	00:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:06
BLANK TEST	0.00	00:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:07
BLANK TEST	0.00	00:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:08
BLANK TEST	0.00	00:09

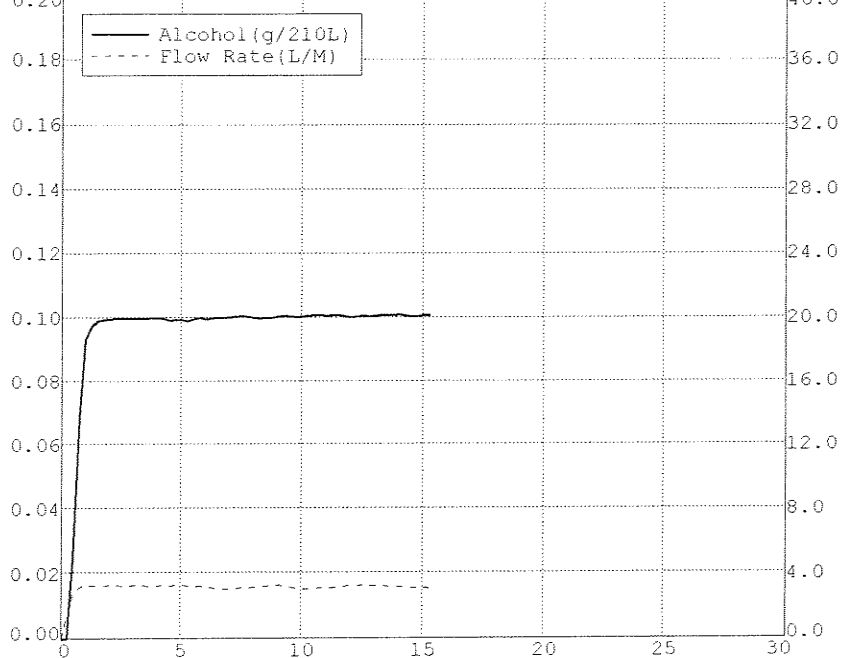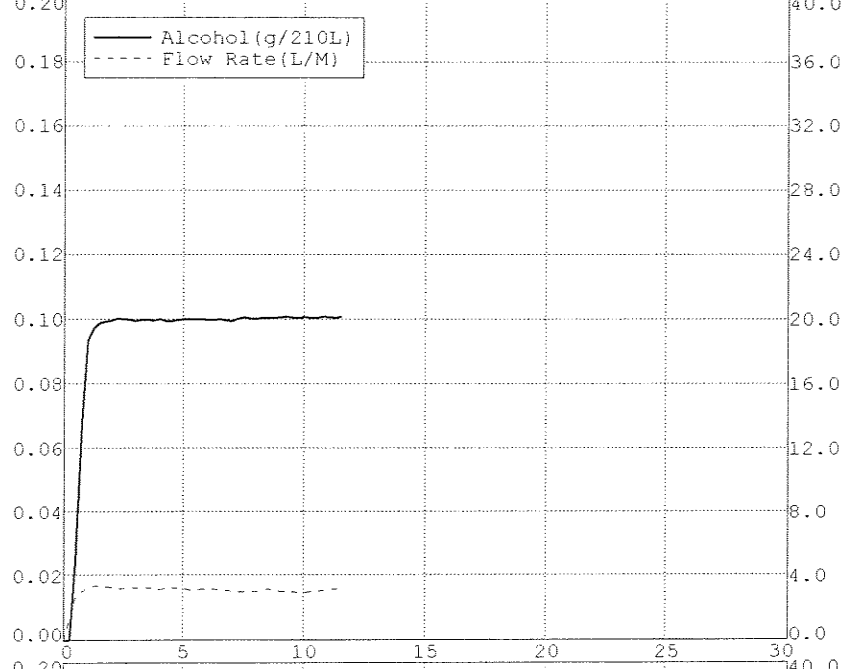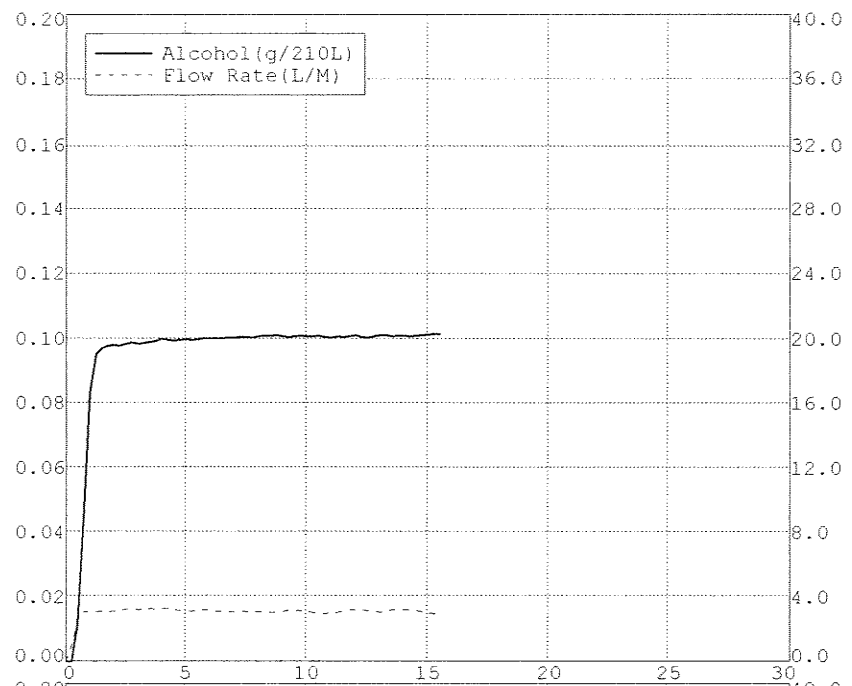

SG- Sgt. Bartlett WS 507/100  
05-09-16