

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 06/06/2016

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 16090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:33
INTERNAL STANDARD	VERIFIED	01:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:33
BLANK TEST	0.00	01:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:34
BLANK TEST	0.00	01:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:36
BLANK TEST	0.00	01:37

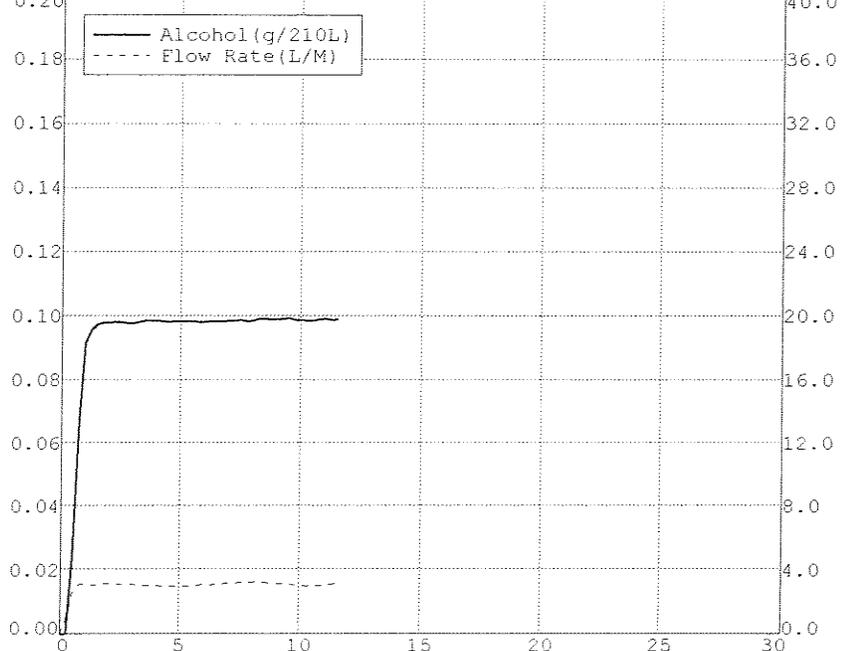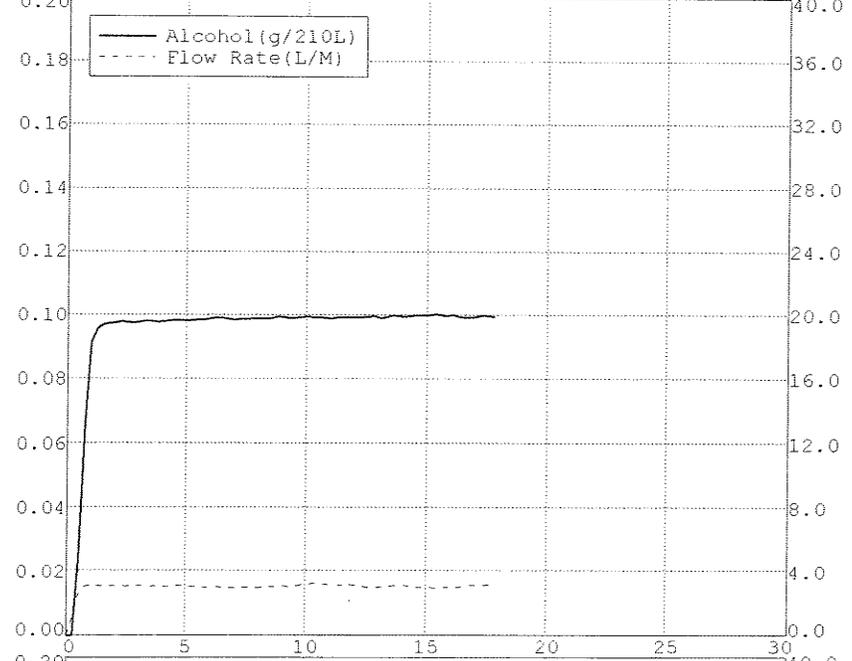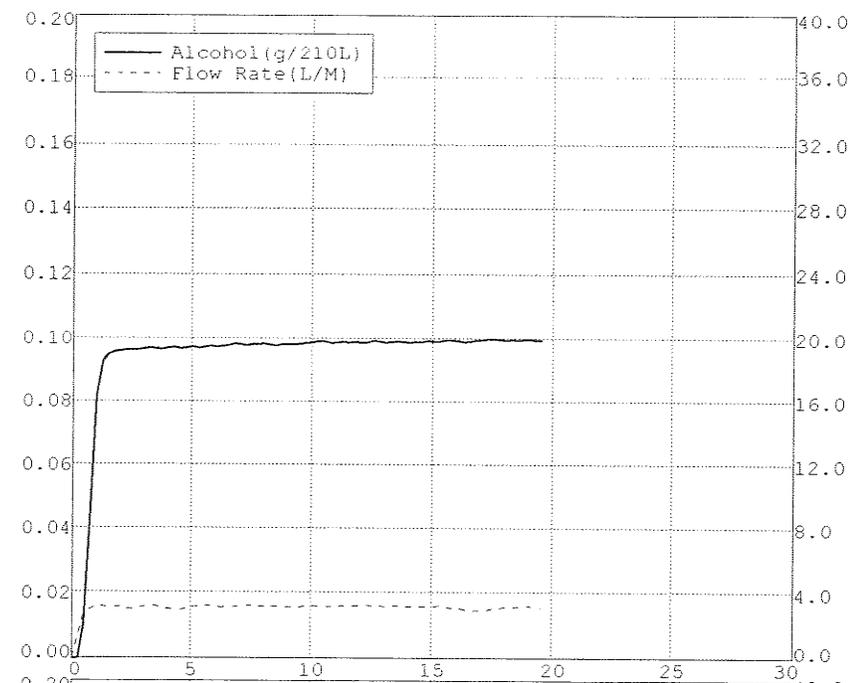

*SOB RJA / [Signature]*  
 WESC #162 06-06-16