

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 06/19/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:31
INTERNAL STANDARD	VERIFIED	01:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:32
BLANK TEST	0.00	01:33
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	01:33
BLANK TEST	0.00	01:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:34
BLANK TEST	0.00	01:35

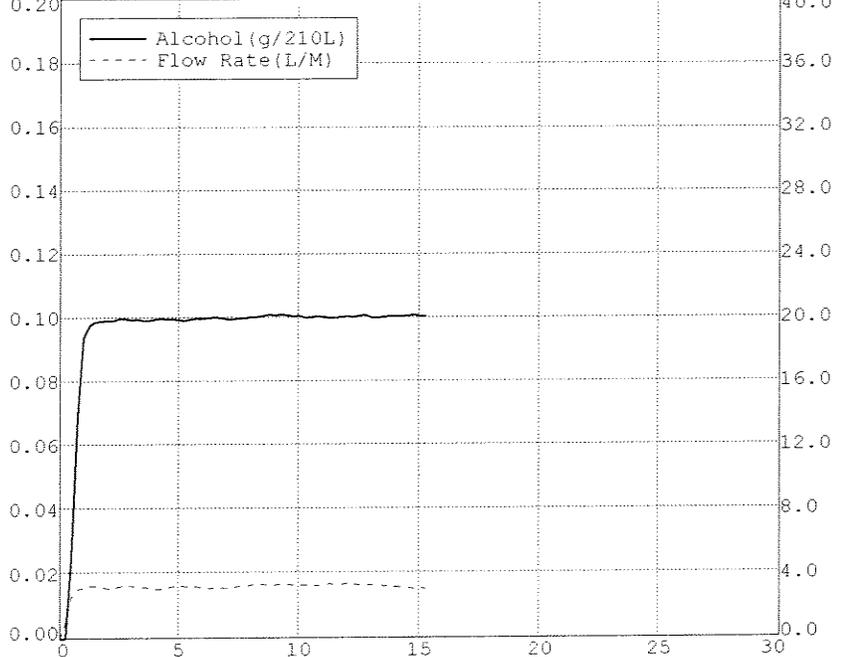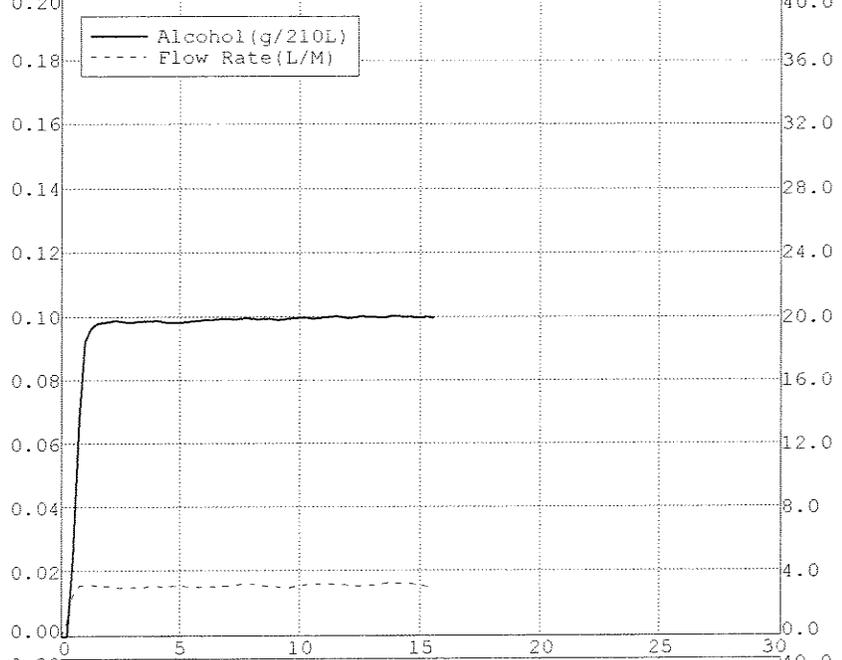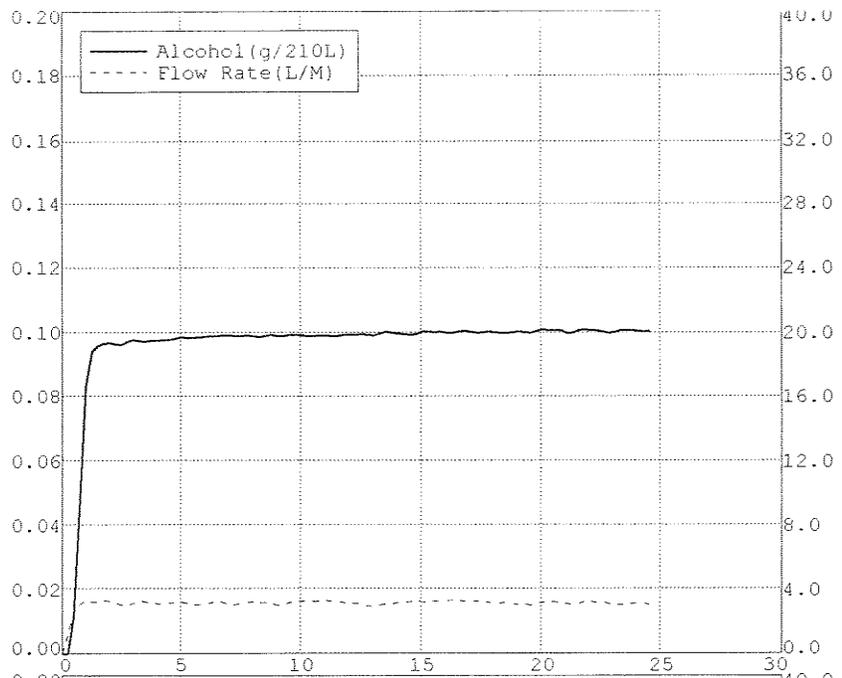

SIS RJA/T... WESU #112  
06-19-16