

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 06/28/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16090

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:47
INTERNAL STANDARD	VERIFIED	01:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	01:47
BLANK TEST	0.00	01:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	01:48
BLANK TEST	0.00	01:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:50
BLANK TEST	0.00	01:51

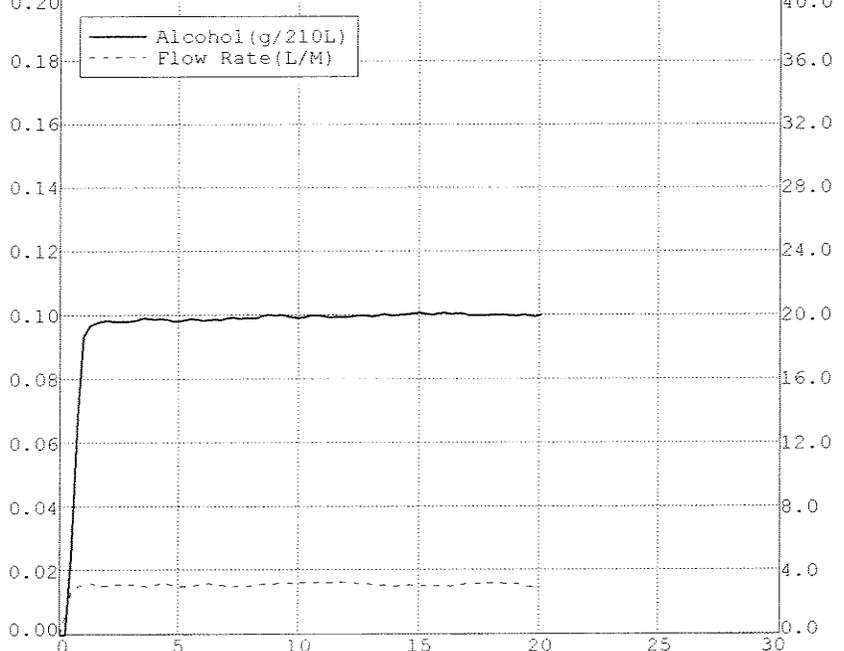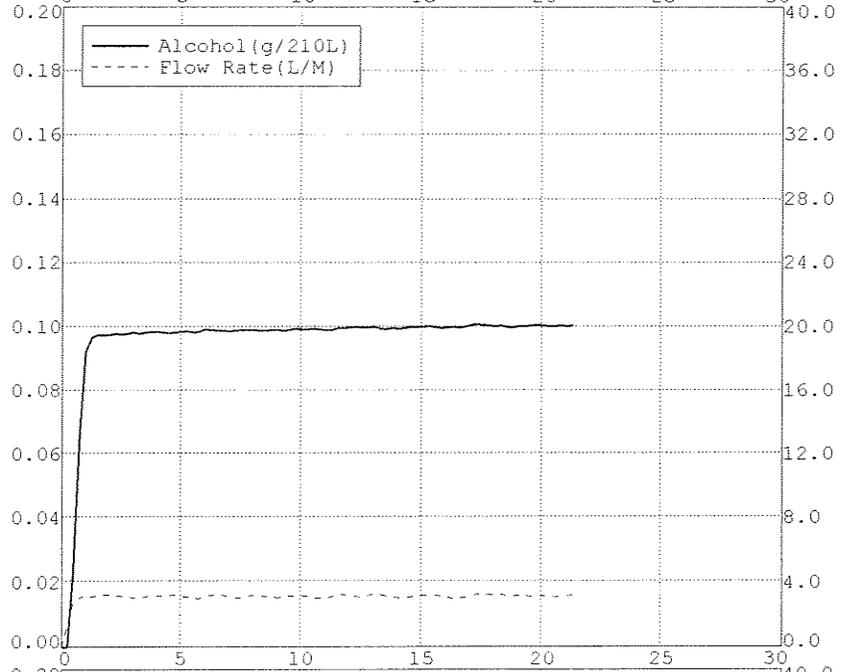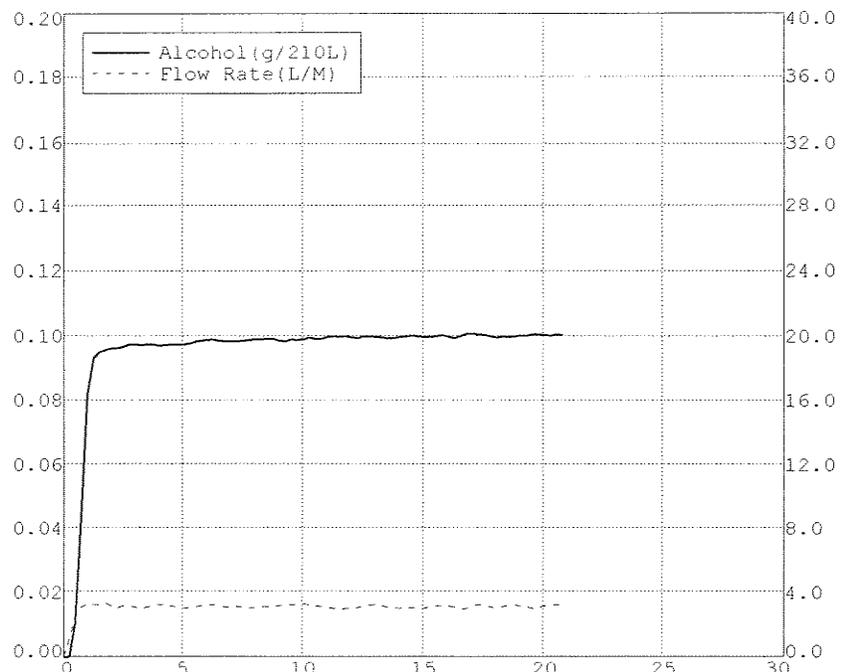

SGS R/J Bartlett WOSO #102
 06-28-16