

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/03/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16090

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:29
INTERNAL STANDARD	VERIFIED	23:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:29
BLANK TEST	0.00	23:30
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:31
BLANK TEST	0.00	23:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:32
BLANK TEST	0.00	23:33

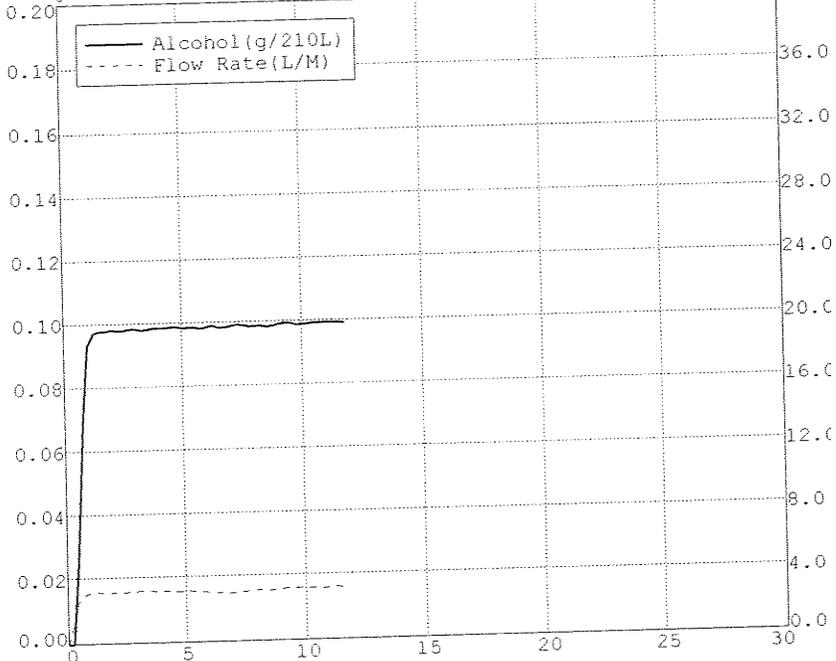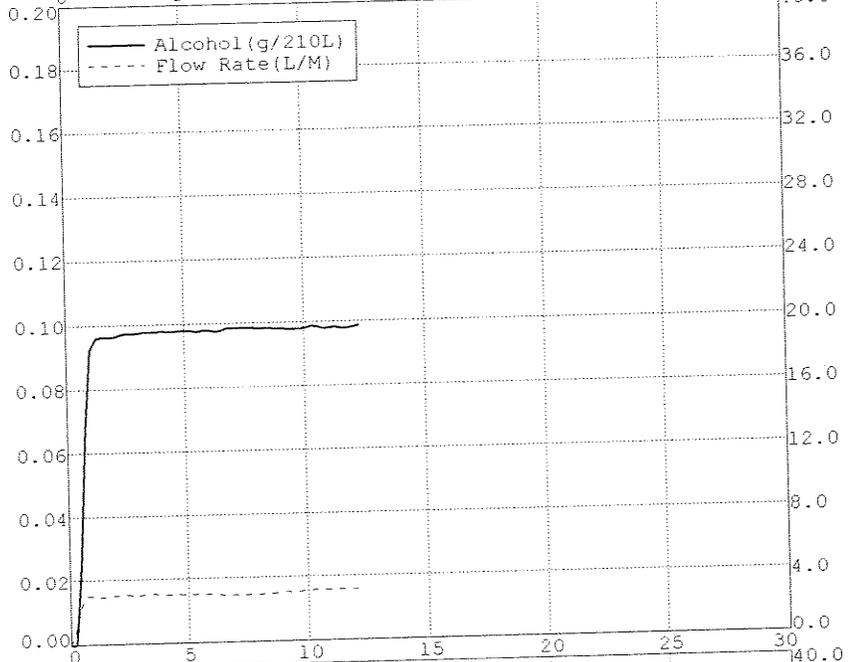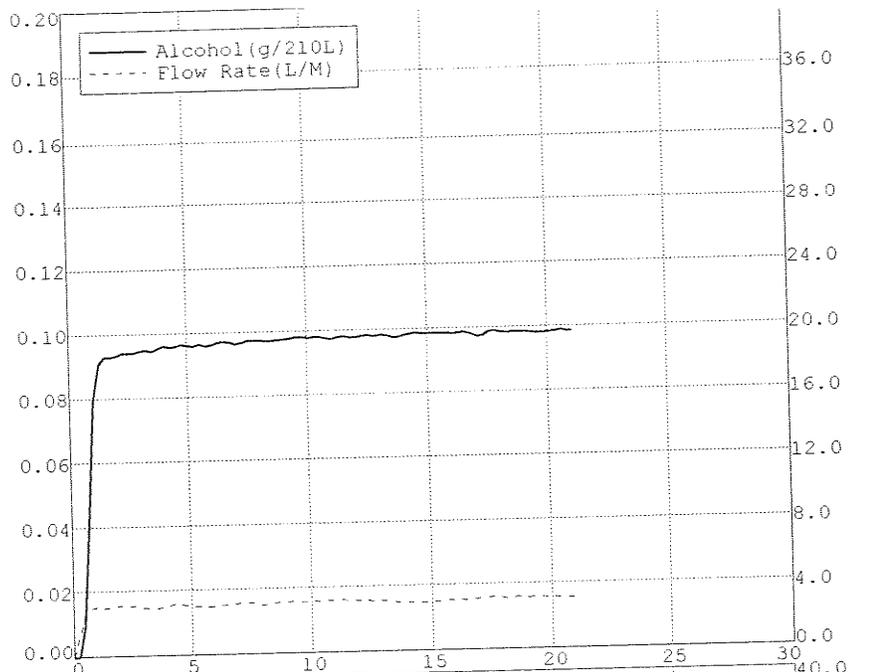

*Sub Sample Bartlett w/ser #162*  
*07-03-16*