

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/25/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16090

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 15:23 |
| INTERNAL STANDARD       | VERIFIED | 15:24 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 15:24 |
| BLANK TEST              | 0.00     | 15:25 |
| REFERENCE STANDARD TEMP | 34.02c   |       |
| REFERENCE STANDARD      | 0.09     | 15:25 |
| BLANK TEST              | 0.00     | 15:26 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 15:27 |
| BLANK TEST              | 0.00     | 15:27 |

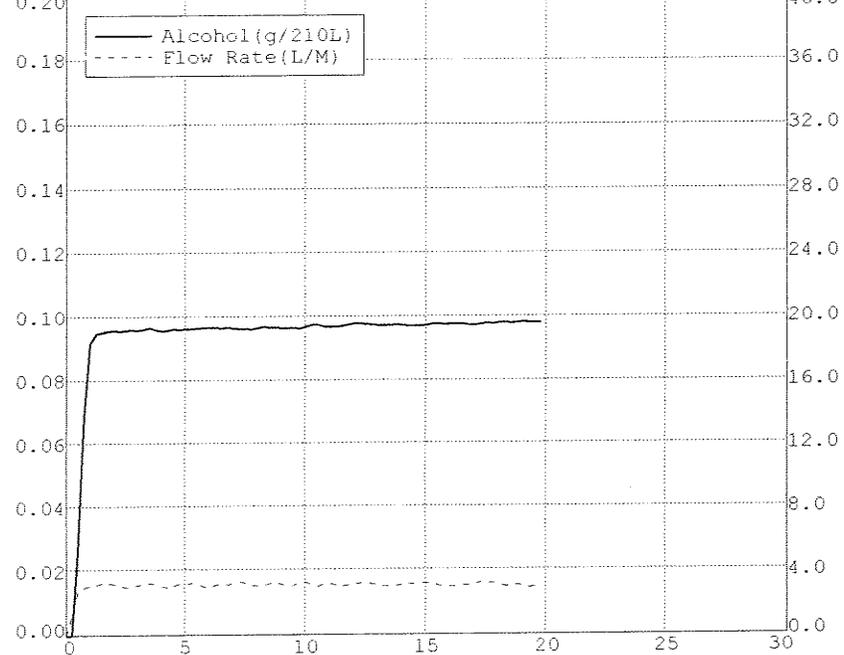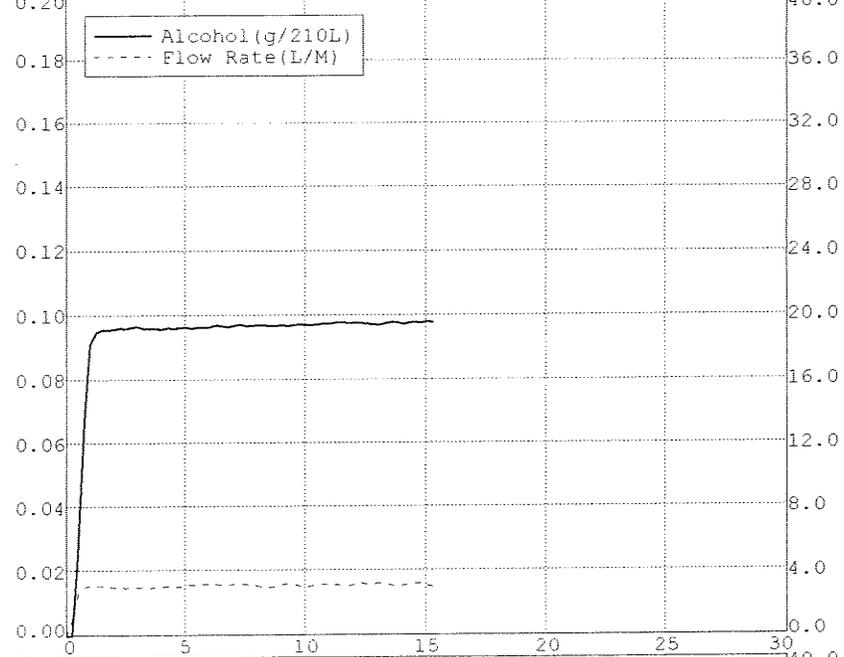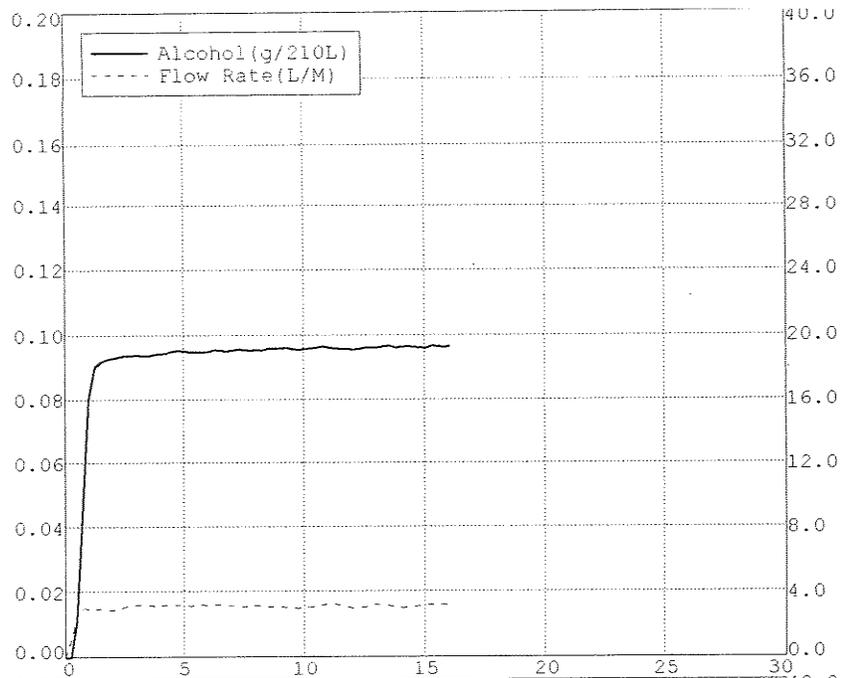

SGT R.J. Bartlett  
WCSO #100 07/25/16