

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/23/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:03
INTERNAL STANDARD	VERIFIED	03:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:04
BLANK TEST	0.00	03:05
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:05
BLANK TEST	0.00	03:06
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	03:06
BLANK TEST	0.00	03:07

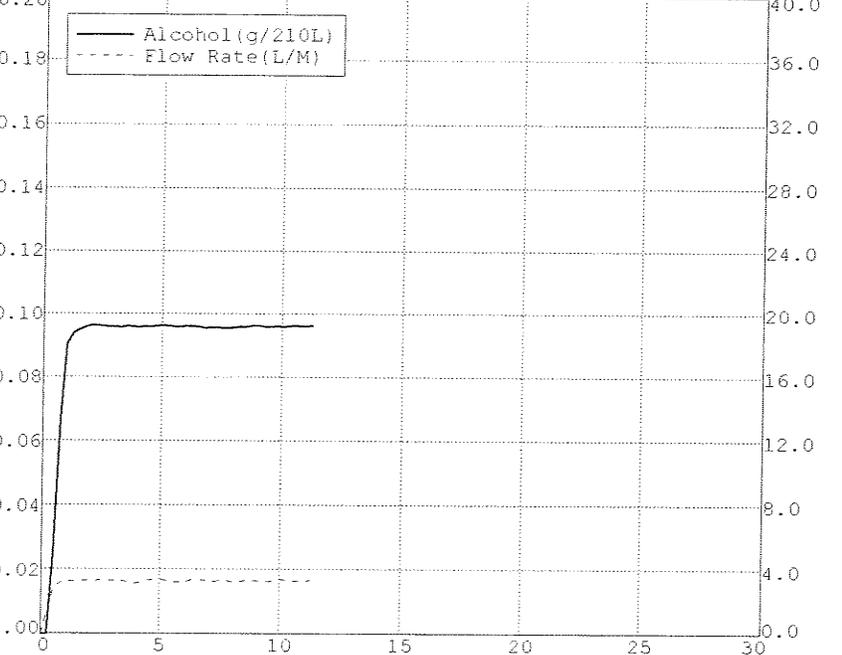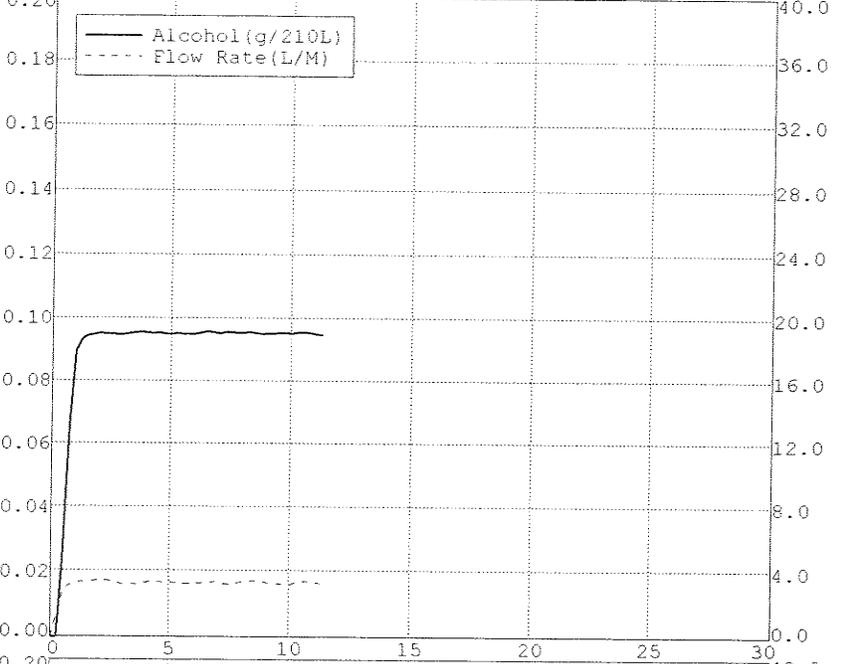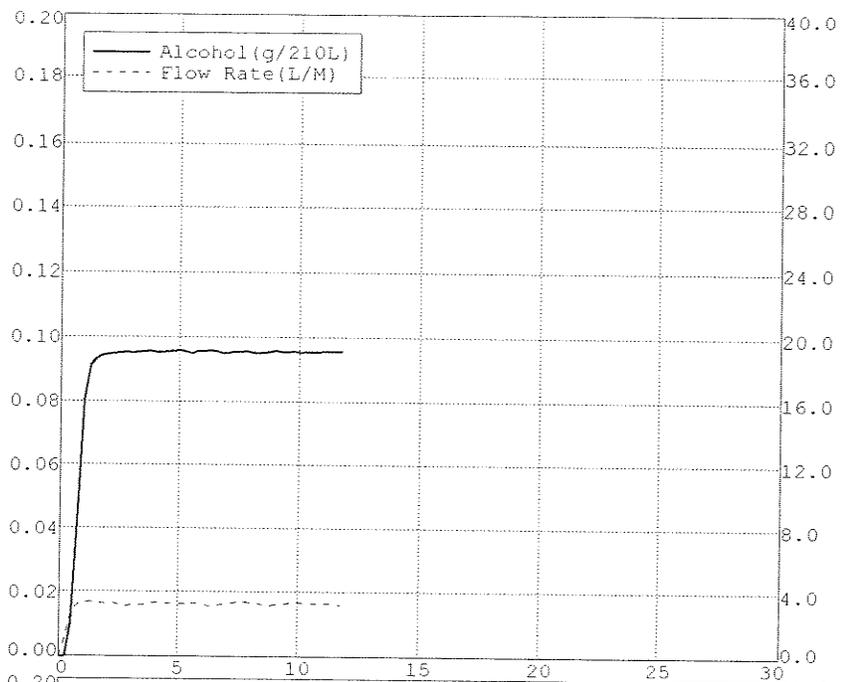

Sus Red of Bartlett WPSO #162

08-23-16