

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 08/29/2016

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:17
INTERNAL STANDARD	VERIFIED	00:17
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:18
BLANK TEST	0.00	00:19
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:19
BLANK TEST	0.00	00:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:20
BLANK TEST	0.00	00:21

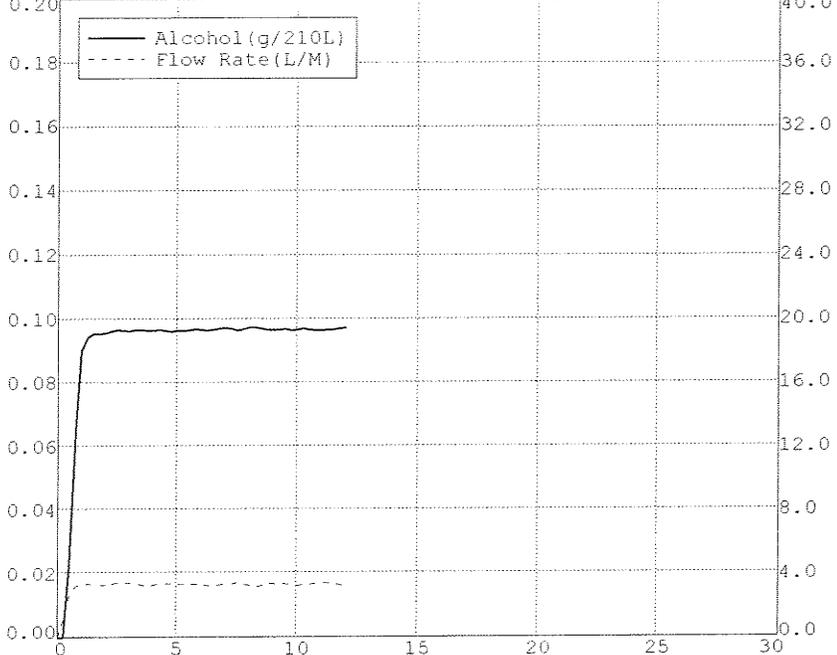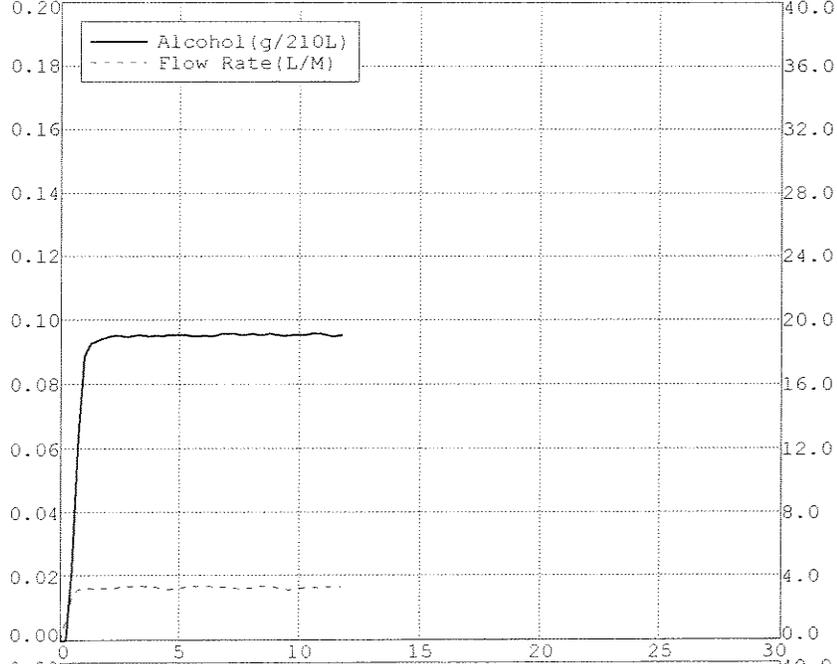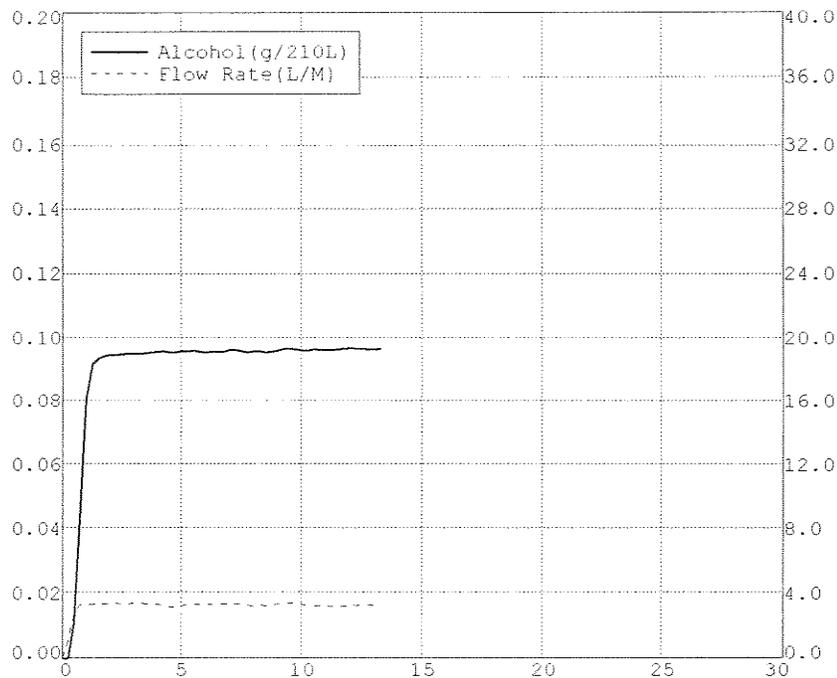

*See RJB Bartlett work #162  
08-29-16*