

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/07/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:20
INTERNAL STANDARD	VERIFIED	00:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:21
BLANK TEST	0.00	00:22
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:22
BLANK TEST	0.00	00:23
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:23
BLANK TEST	0.00	00:24

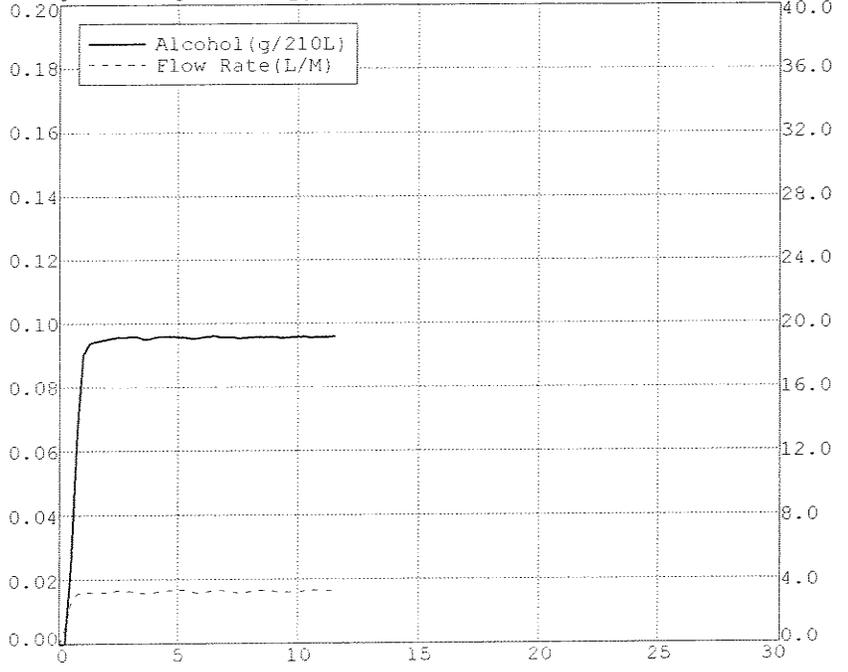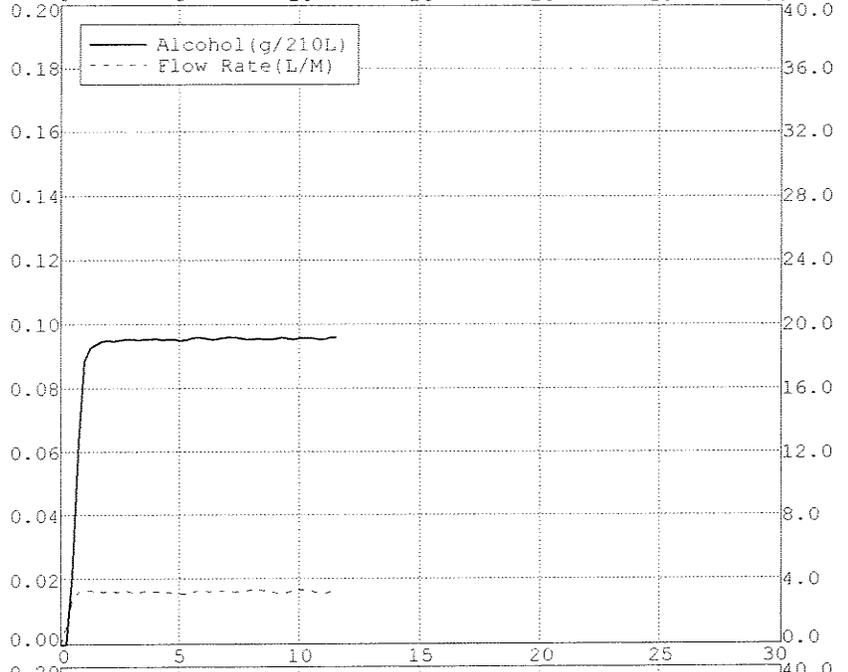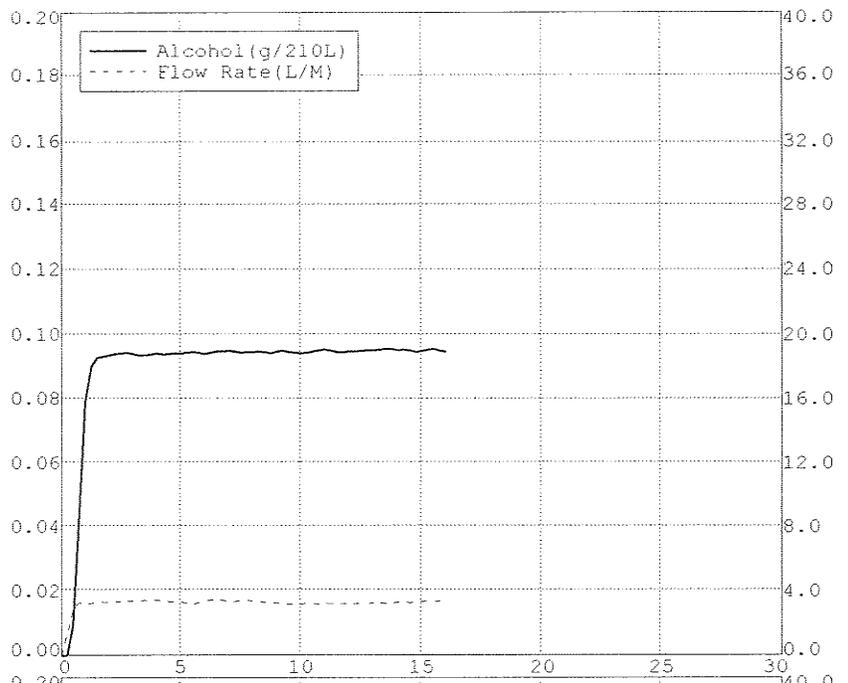

SGS Analytical Services *Warren #162*
09-07-16