

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 09/12/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:40
INTERNAL STANDARD	VERIFIED	00:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:40
BLANK TEST	0.00	00:41
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:42
BLANK TEST	0.00	00:42
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:43
BLANK TEST	0.00	00:44

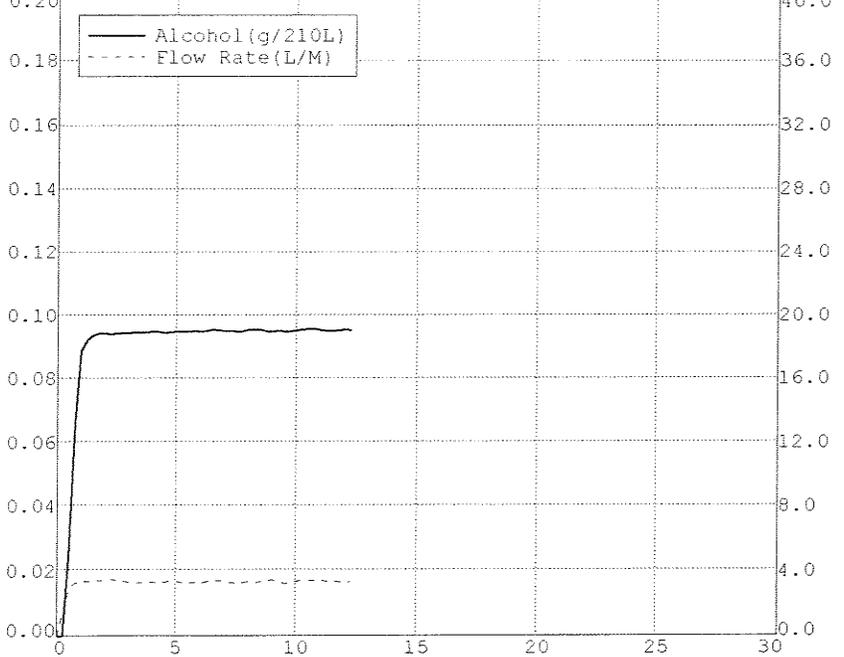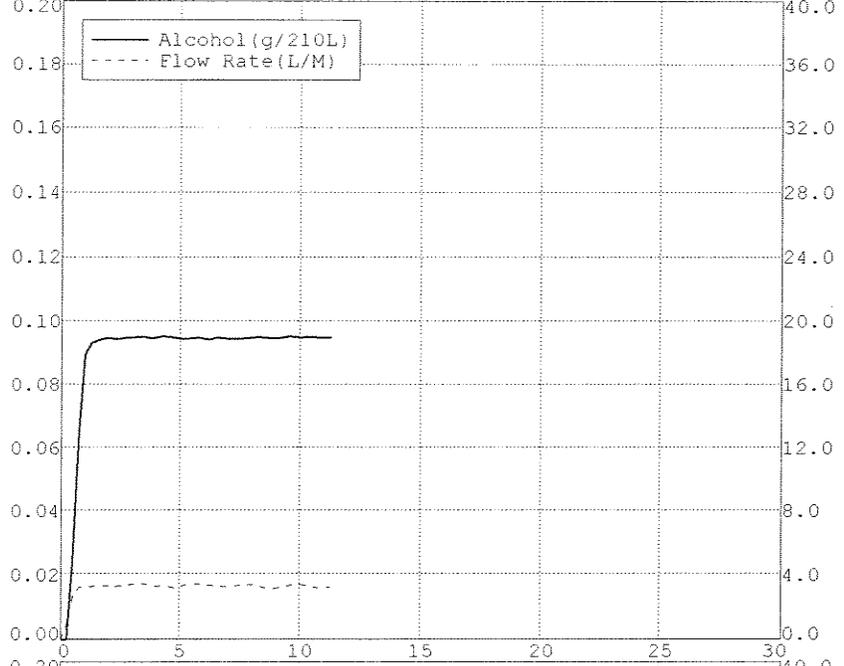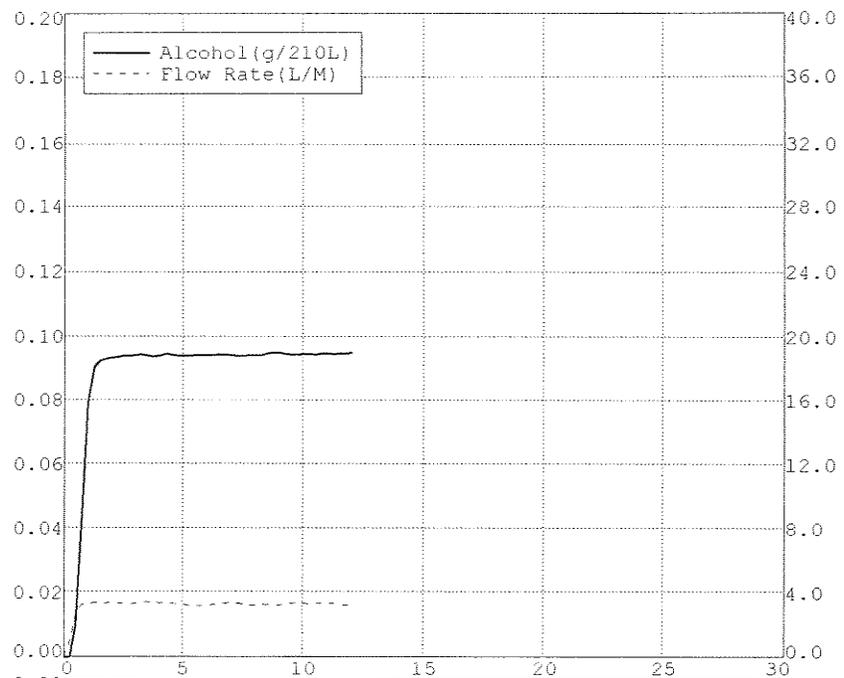

Sgt Ralph J Bartlett WOSU #162
 09-12-16