

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/25/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:18
INTERNAL STANDARD	VERIFIED	22:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:18
BLANK TEST	0.00	22:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:19
BLANK TEST	0.00	22:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	22:21
BLANK TEST	0.00	22:22

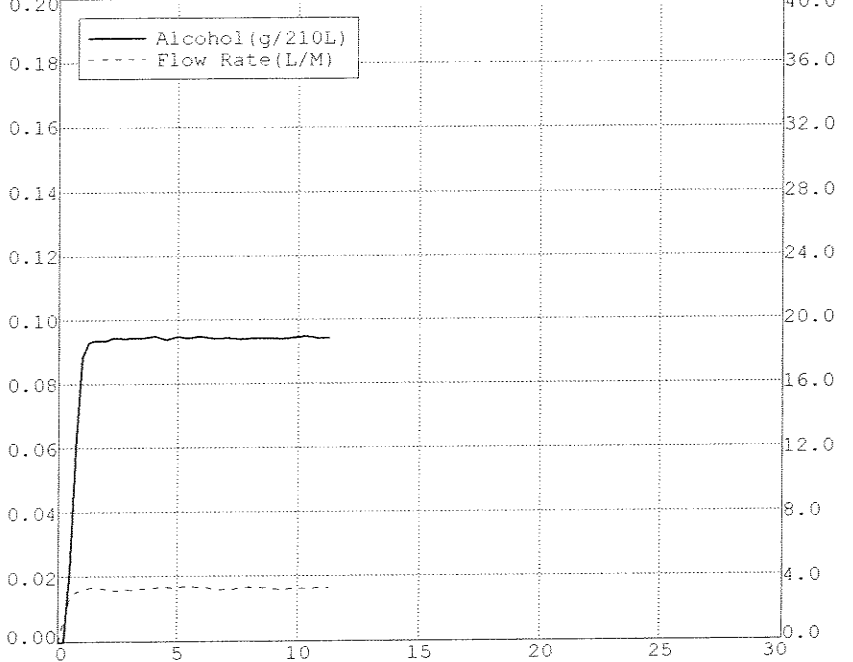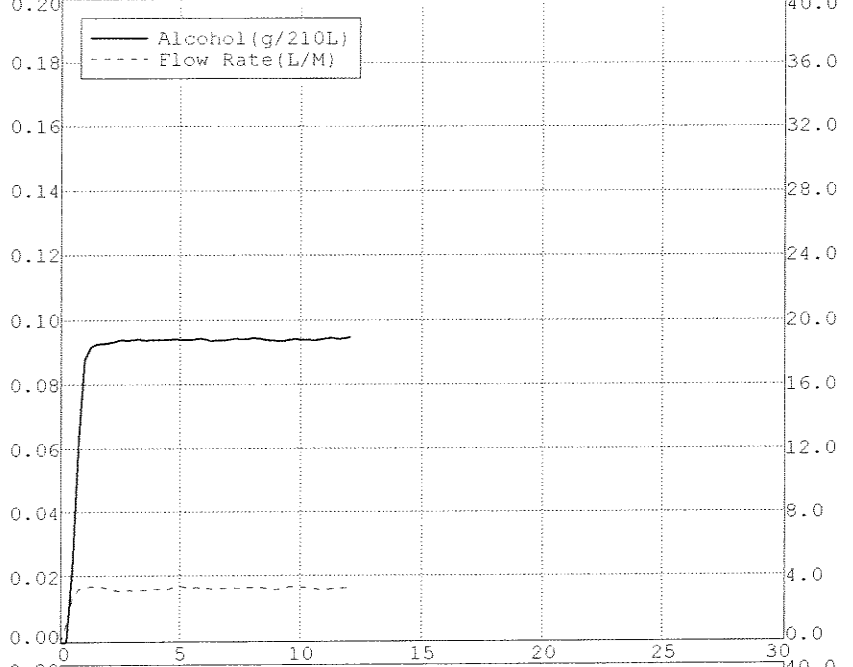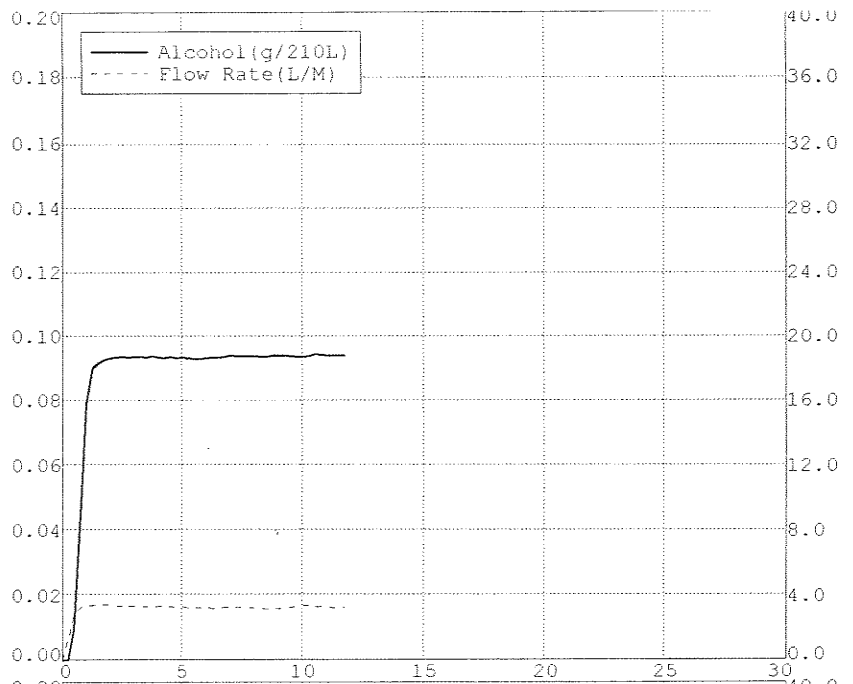

SG *RJ Bartlett* case #162
09-25-16