

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 10/18/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:32
INTERNAL STANDARD	VERIFIED	01:32
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:33
BLANK TEST	0.00	01:33
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:34
BLANK TEST	0.00	01:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:35
BLANK TEST	0.00	01:36

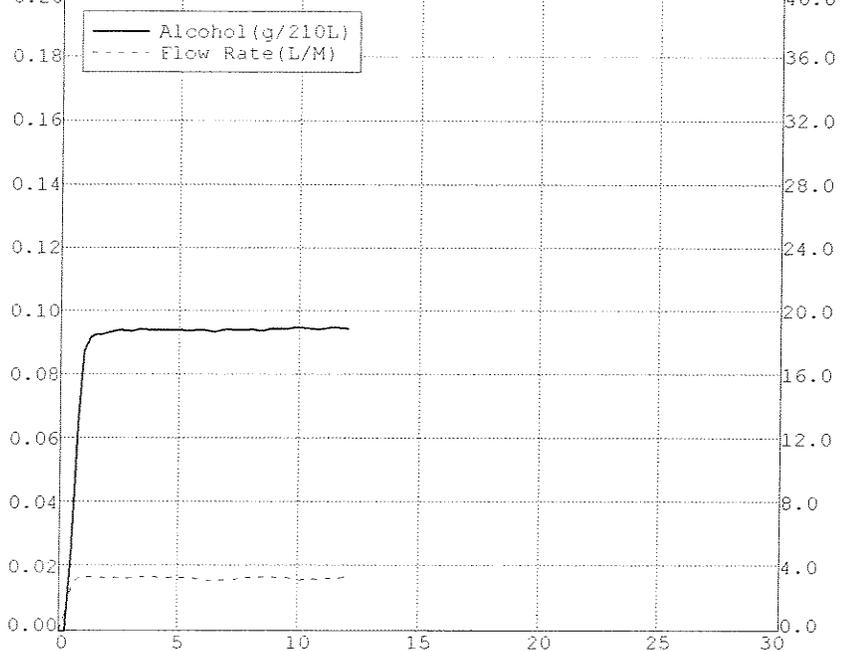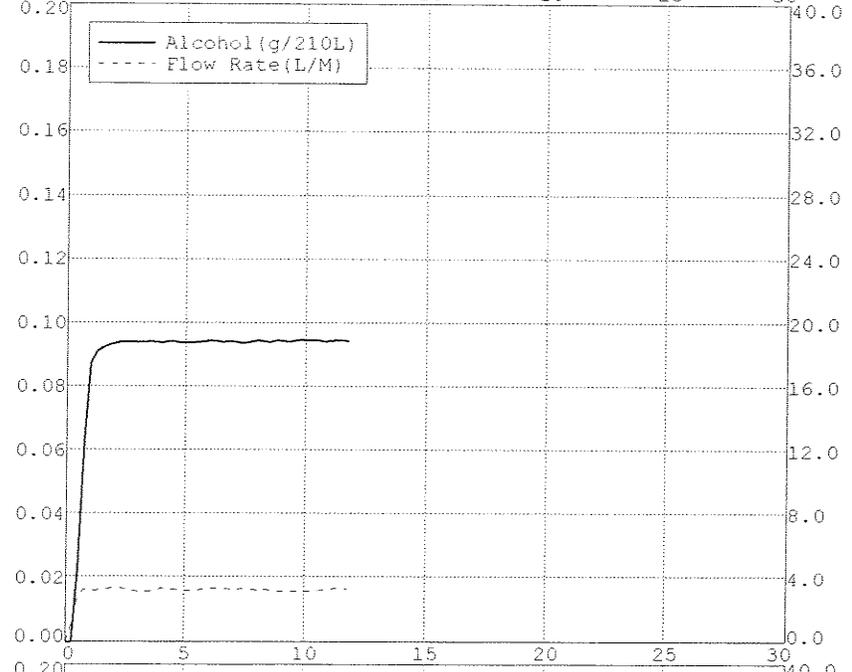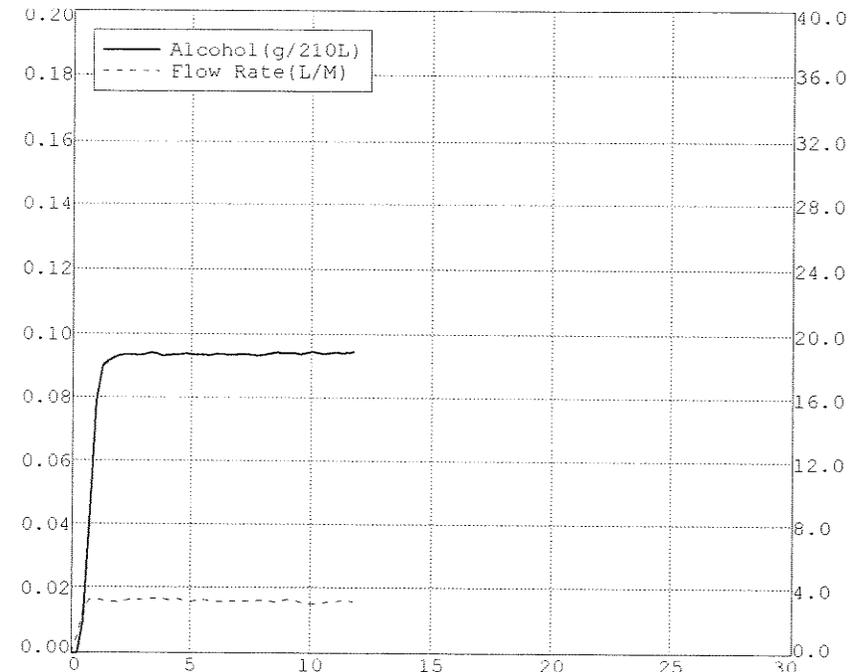

Sgt R. J. Bartlett WOSO #142
 10-18-16