

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/24/2016

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:23
INTERNAL STANDARD	VERIFIED	01:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:23
BLANK TEST	0.00	01:24
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:24
BLANK TEST	0.00	01:25
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:26
BLANK TEST	0.00	01:27

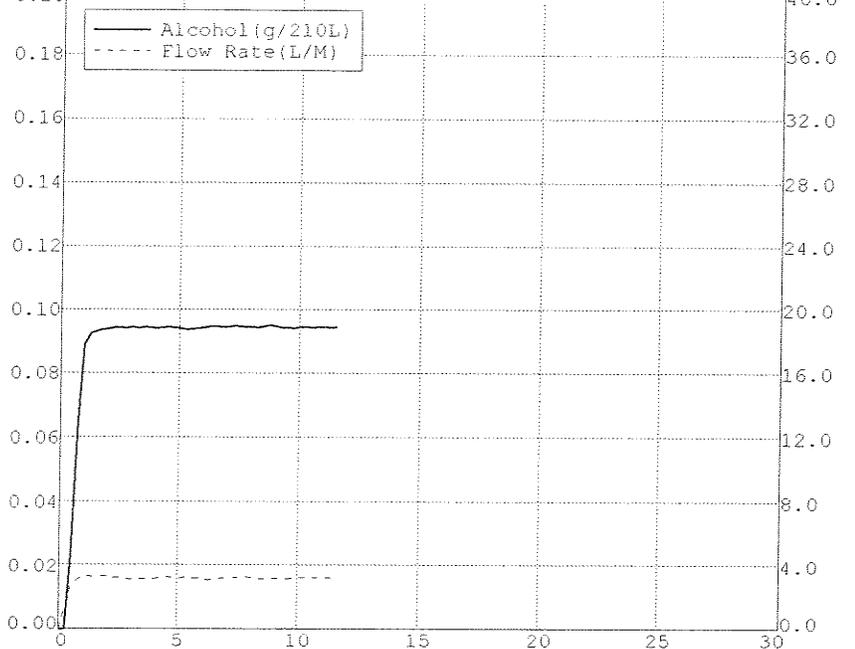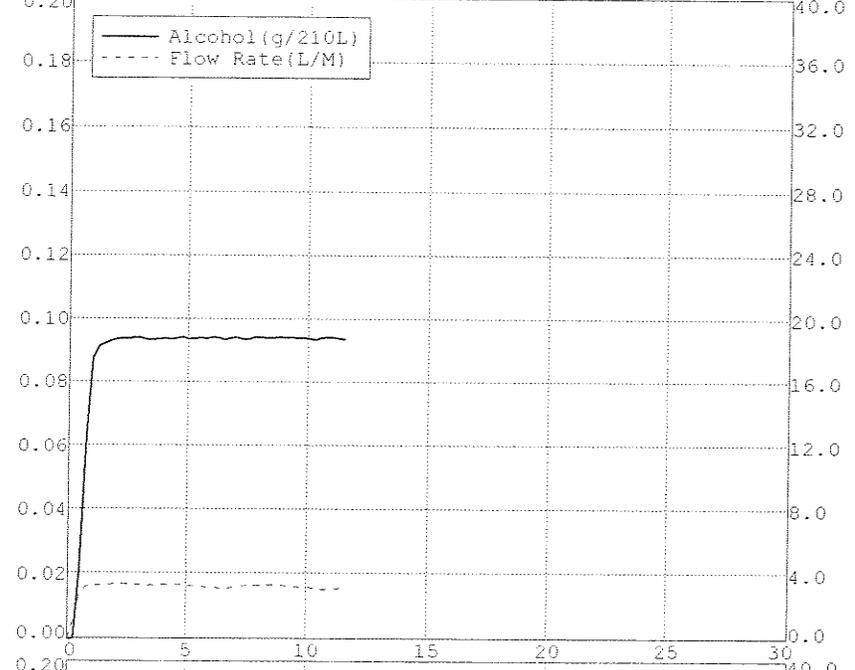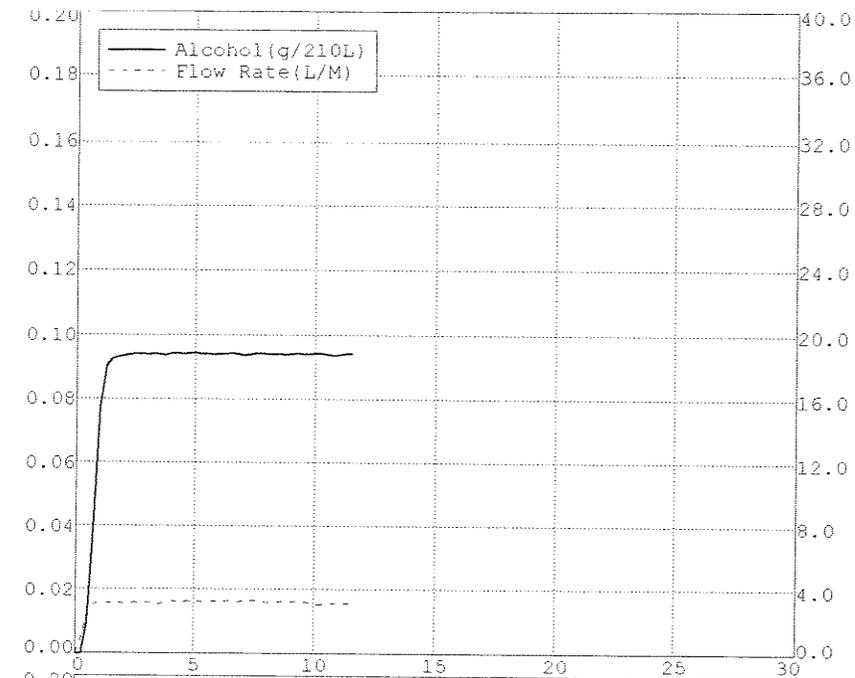

*See Ralph Bartlett work #100
10-24-16*