

SUPERVISOR TEST



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/07/2016

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:42
INTERNAL STANDARD	VERIFIED	12:42
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	12:42
BLANK TEST	0.00	12:43
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	12:43
BLANK TEST	0.00	12:44
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	12:44
BLANK TEST	0.00	12:45

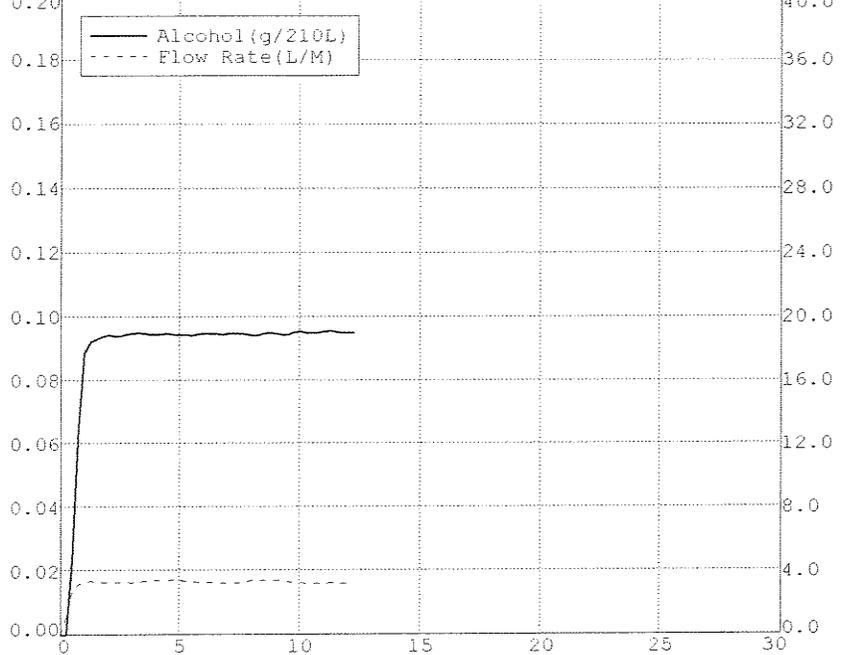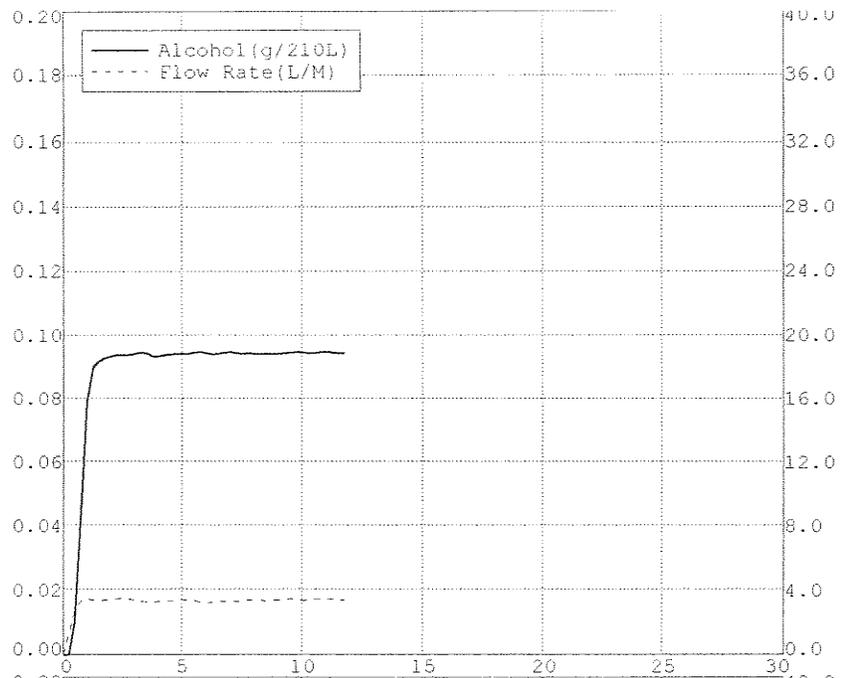

C. B. Geisler #245 11/07/16