

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/21/2016

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:35
INTERNAL STANDARD	VERIFIED	10:35
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	10:35
BLANK TEST	0.00	10:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:37
BLANK TEST	0.00	10:37
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	10:38
BLANK TEST	0.00	10:39

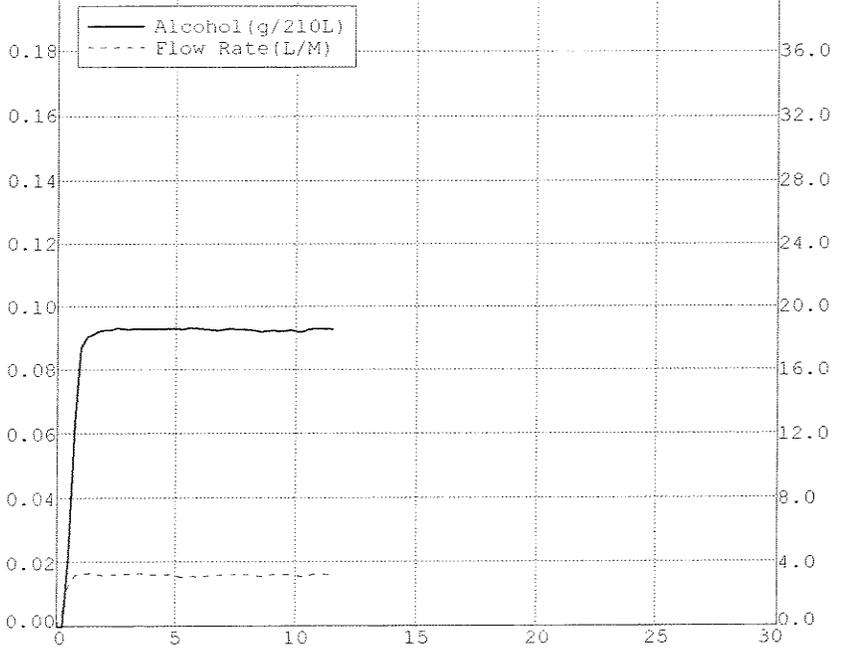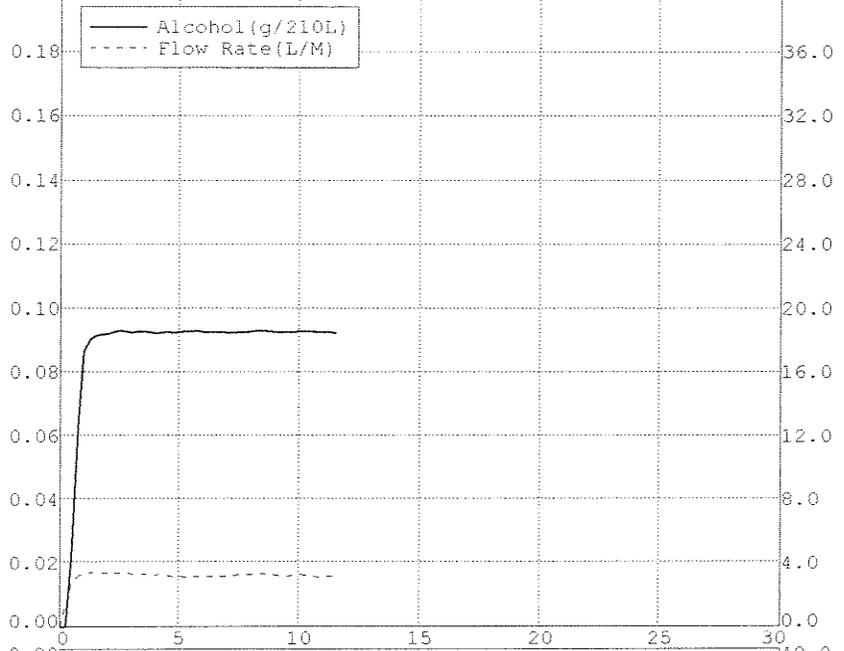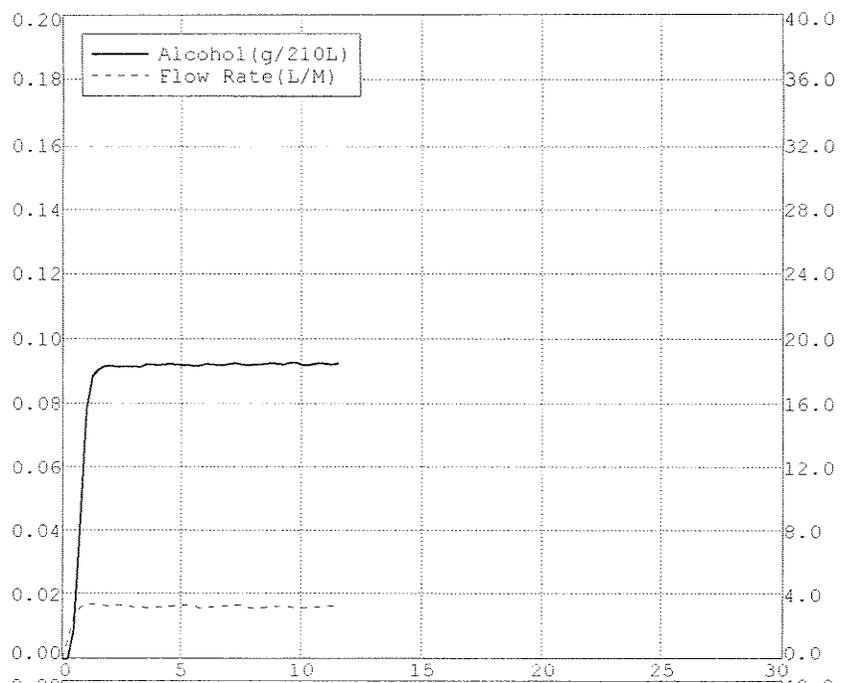

Charles B. Geisler #244