

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 12/05/2016

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:01
INTERNAL STANDARD	VERIFIED	00:01
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:02
BLANK TEST	0.00	00:03
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:03
BLANK TEST	0.00	00:04
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	00:04
BLANK TEST	0.00	00:05

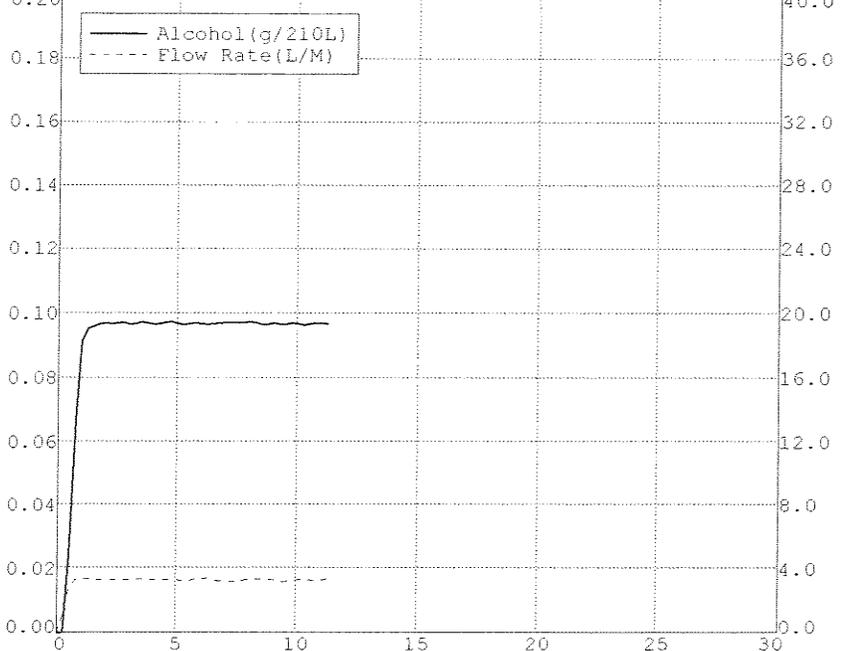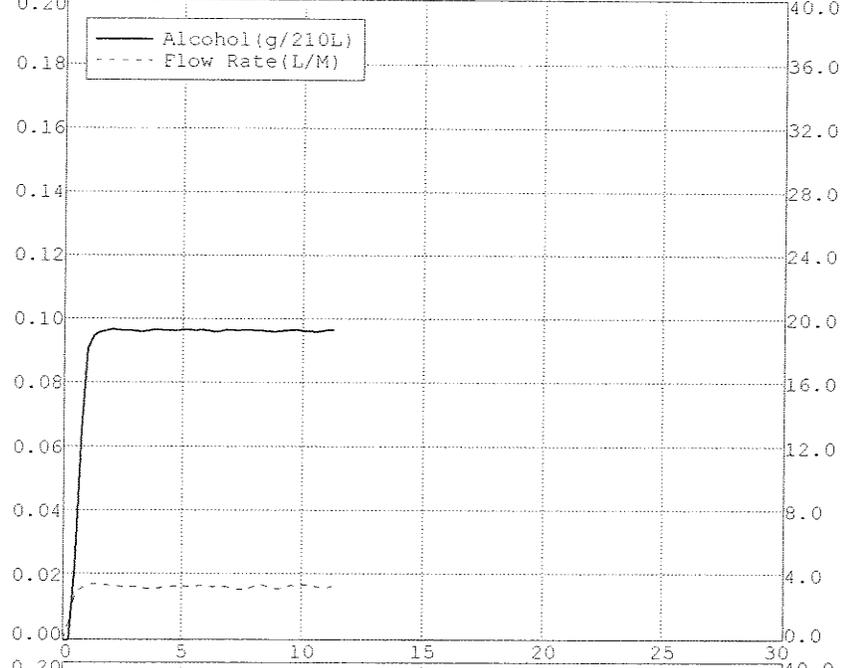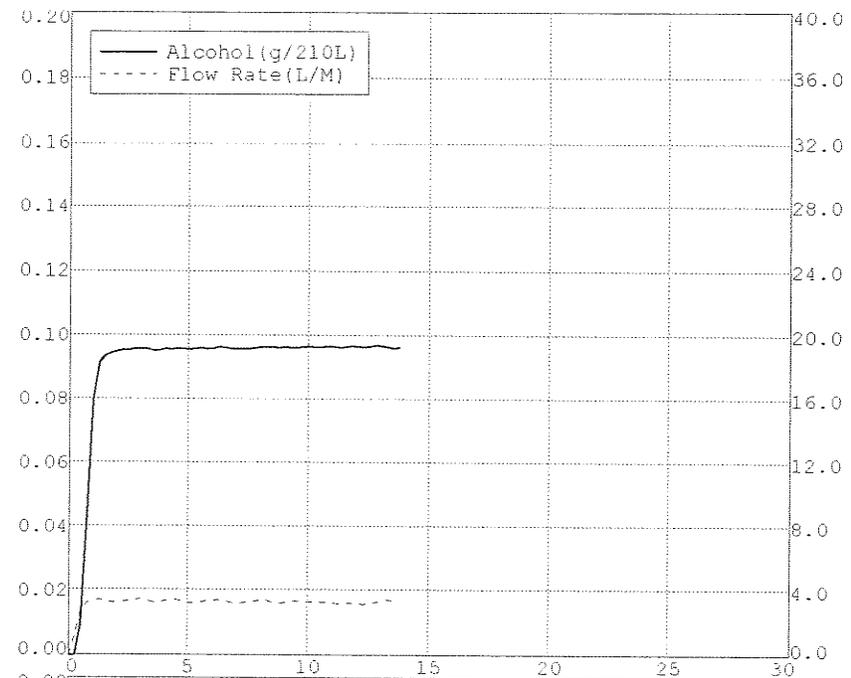

SEE 8/17 Runway WCSO #162  
 12-5-16