

SUPERVISOR TEST



WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 03/18/2016

OPERATOR NAME:
 RALPH J BARTLETT
 Permit #: 26222
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 15250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:10
INTERNAL STANDARD	VERIFIED	02:10
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	02:10
BLANK TEST	0.00	02:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:11
BLANK TEST	0.00	02:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:13
BLANK TEST	0.00	02:14

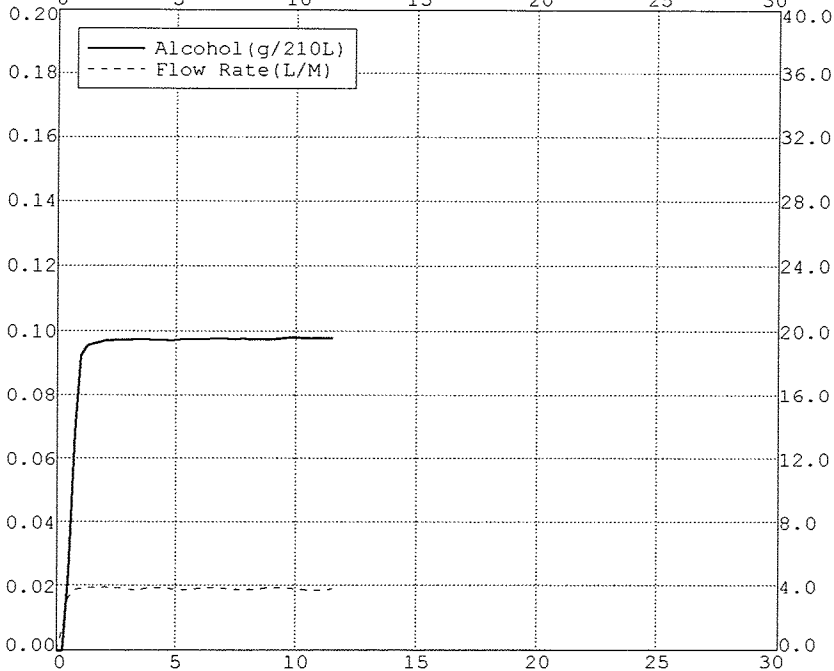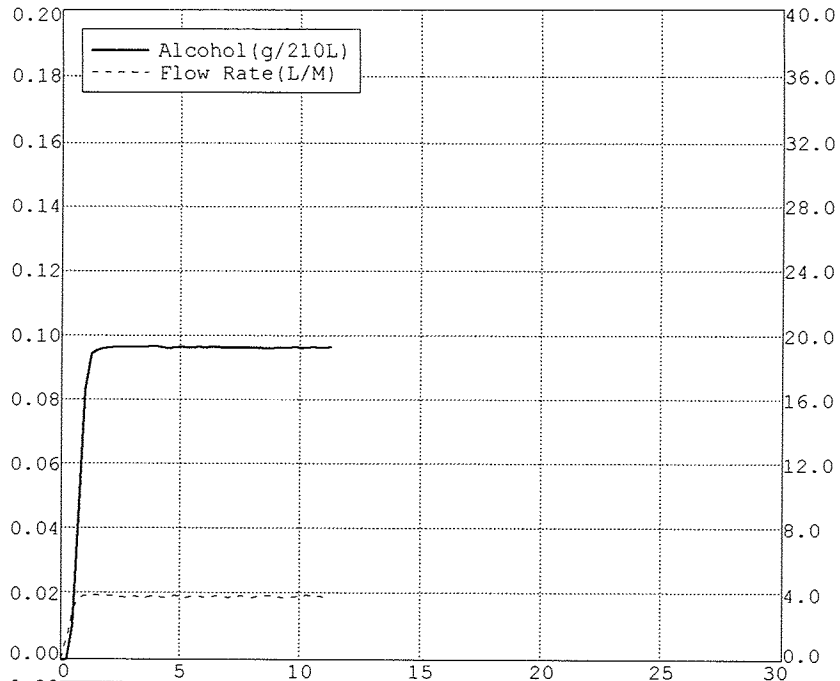

SL5 R/J
 Runway weio #162
 03-18-16