

SOLUTION CHANGE




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 08/15/2016

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:36
INTERNAL STANDARD	VERIFIED	15:36
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	15:37
BLANK TEST	0.00	15:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	15:38
BLANK TEST	0.00	15:39
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	15:39
BLANK TEST	0.00	15:40

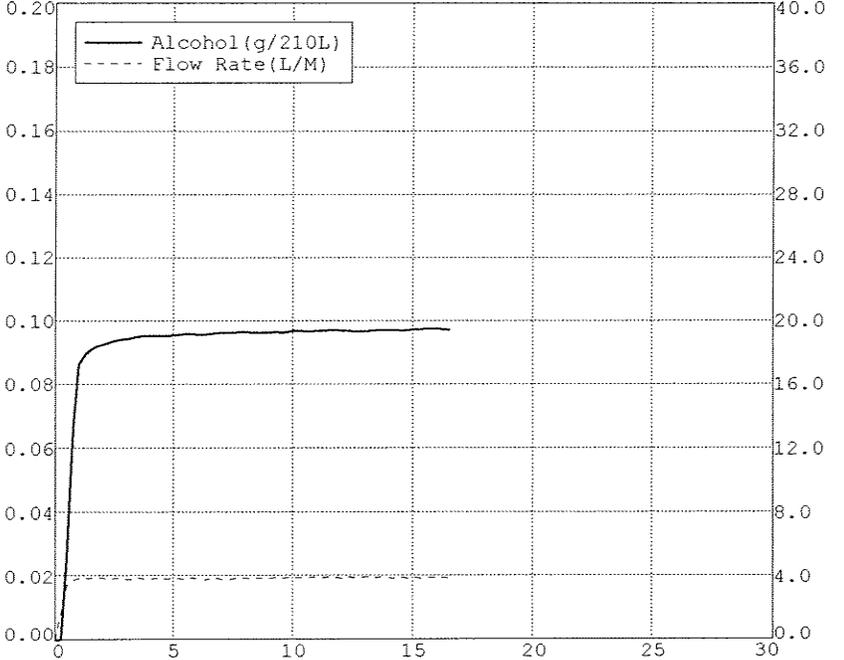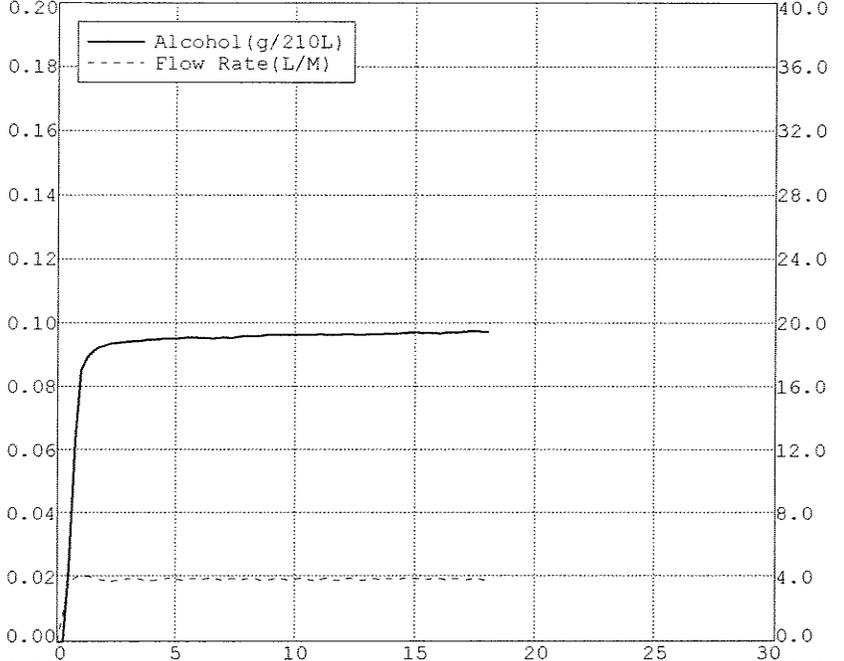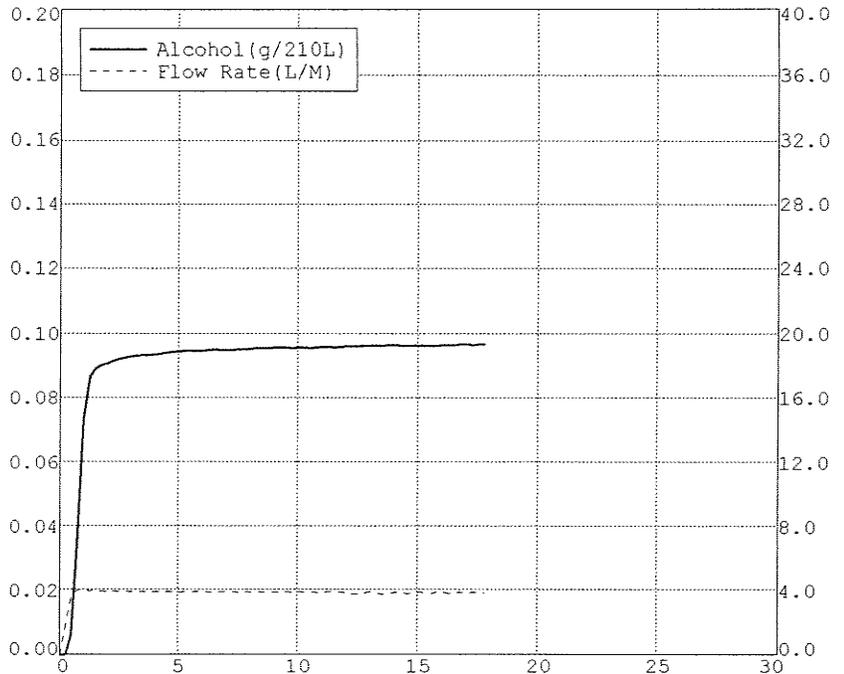

*Charles B. Geisler #248*