

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 09/07/2016

OPERATOR NAME:
RALPH J BARTLET
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16120

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:15
INTERNAL STANDARD	VERIFIED	01:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:15
BLANK TEST	0.00	01:16
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	01:16
BLANK TEST	0.00	01:17
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:17
BLANK TEST	0.00	01:18

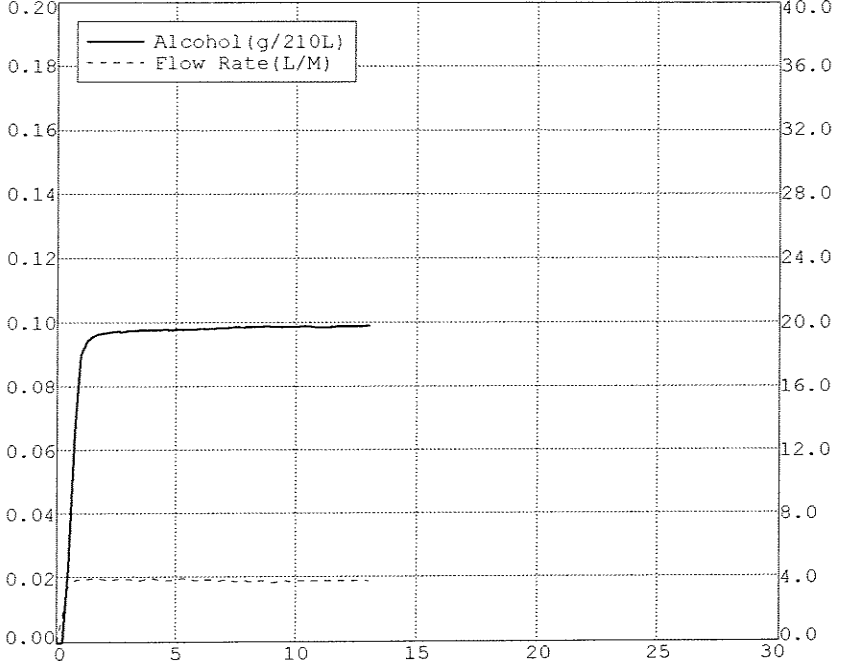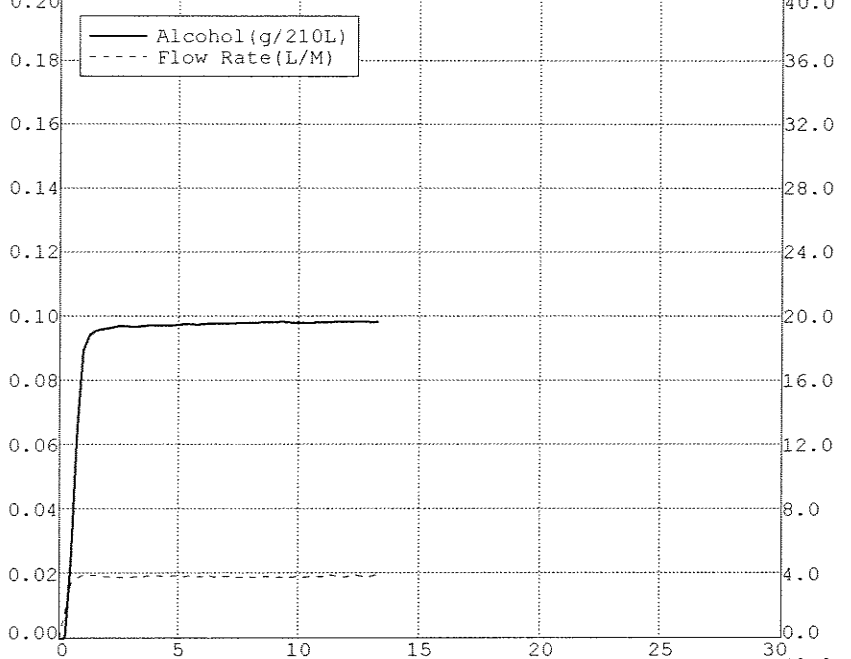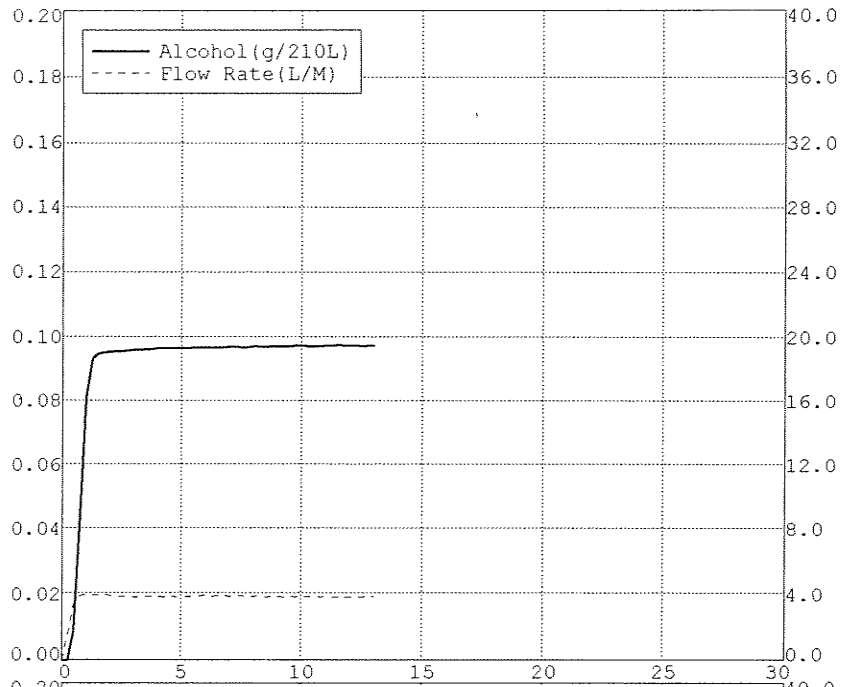

SUS Rel of Th... WCSO #162
09-07-16