

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/07/2016

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:51
INTERNAL STANDARD	VERIFIED	11:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:52
BLANK TEST	0.00	11:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:53
BLANK TEST	0.00	11:54
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:54
BLANK TEST	0.00	11:55

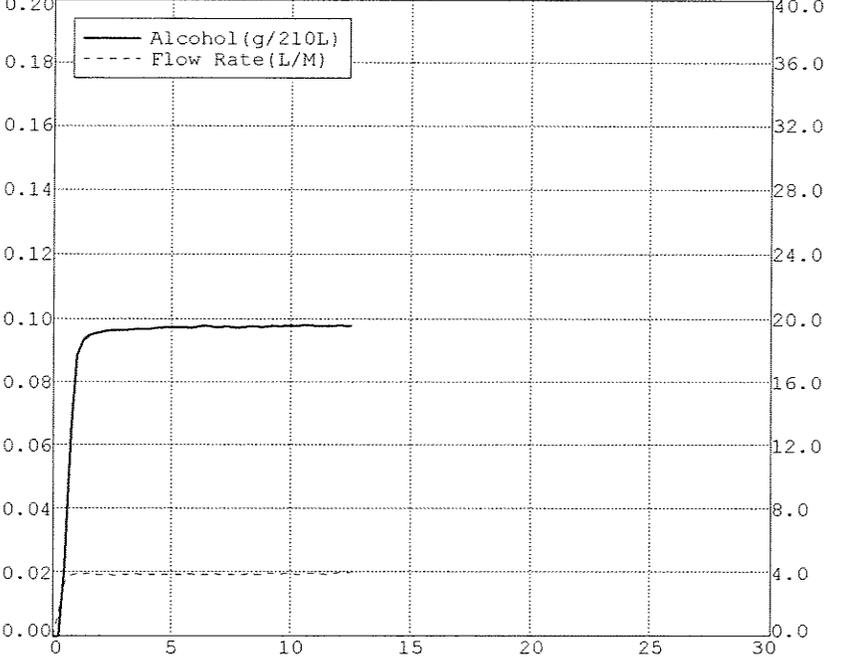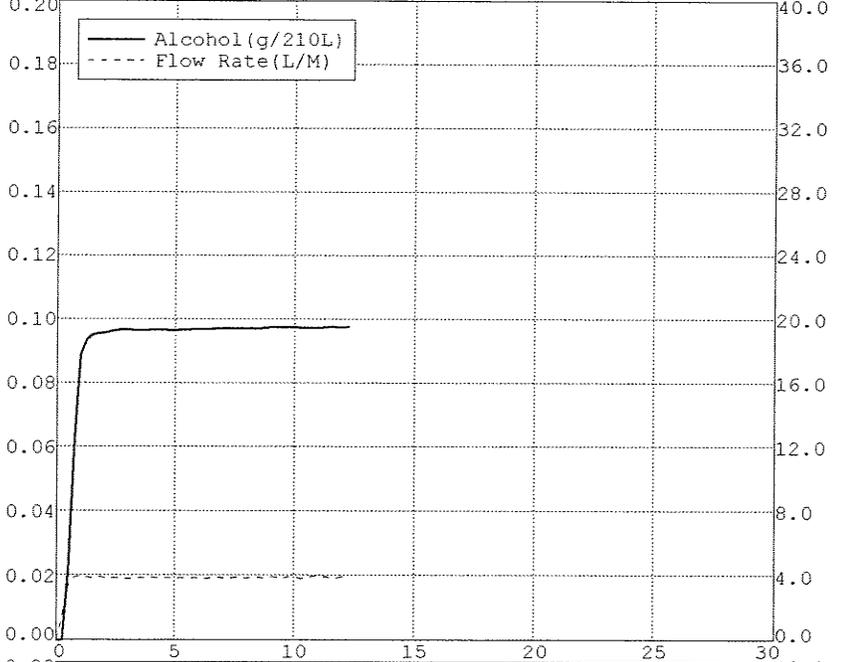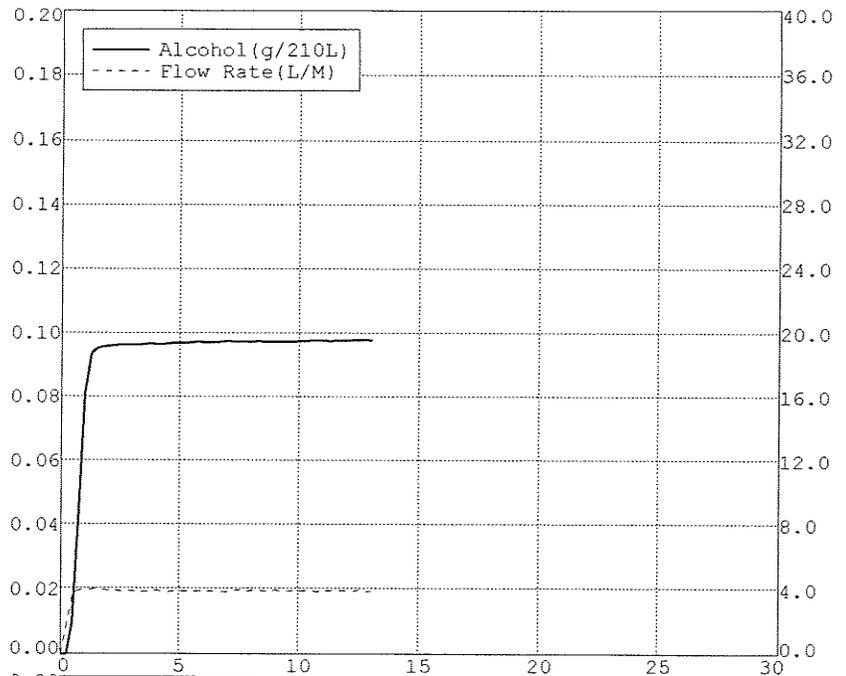

*P. Charles B. Geisler* #248  
11/07/16