

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 11/21/2016

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN COUNTY
SHERIFF'S OFFICE
Reference Standard #: 16170

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:45
INTERNAL STANDARD	VERIFIED	09:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:45
BLANK TEST	0.00	09:46
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	09:47
BLANK TEST	0.00	09:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	09:48
BLANK TEST	0.00	09:49

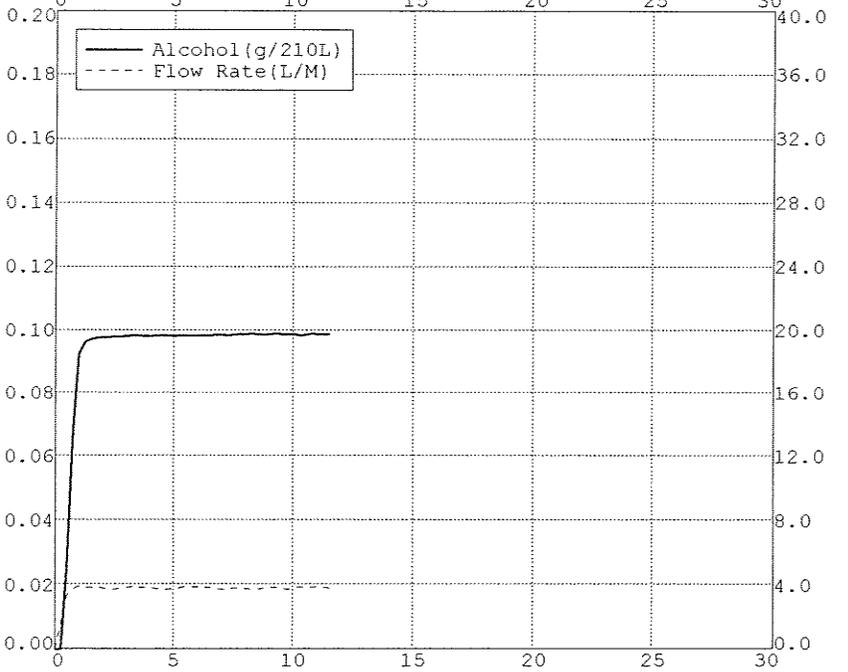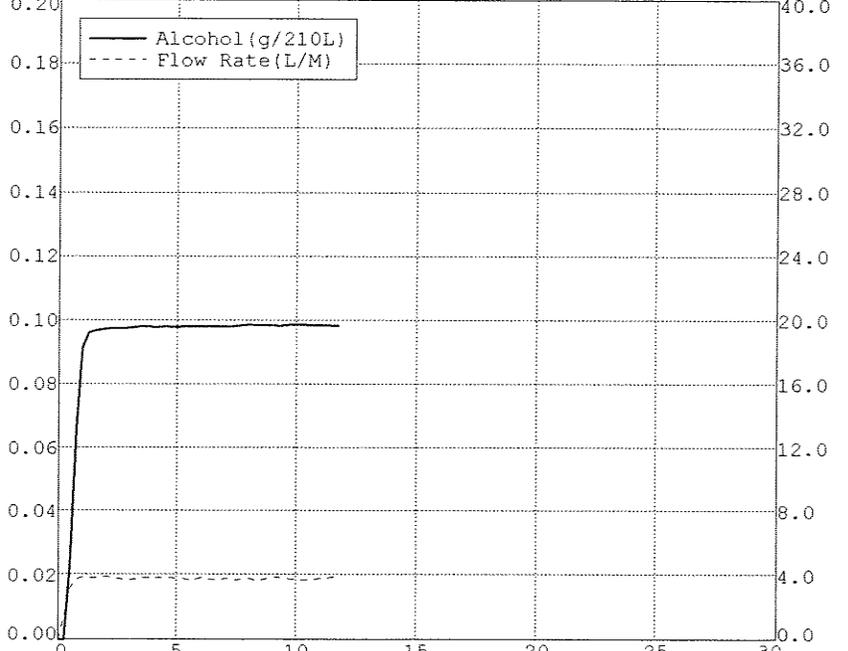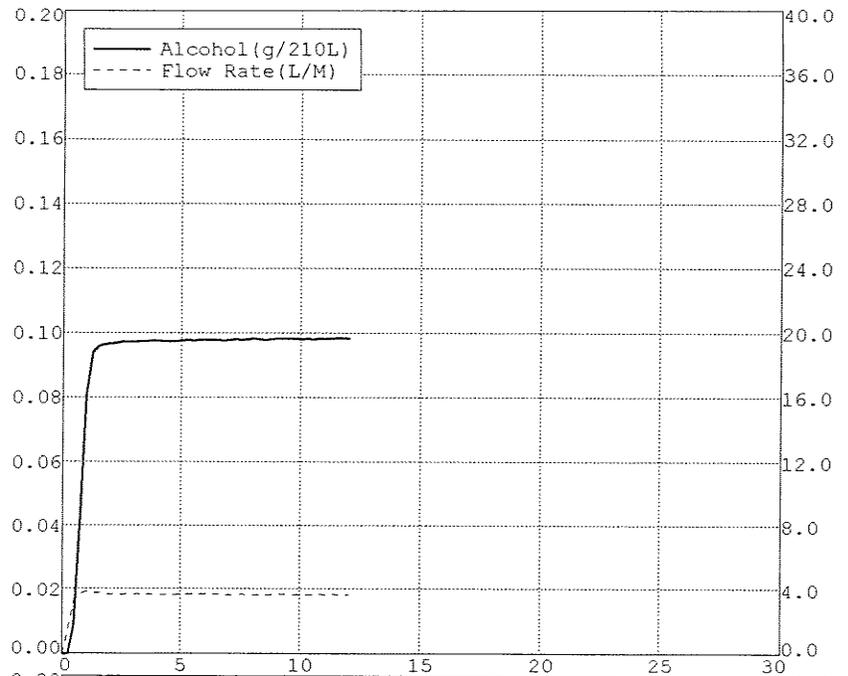

Charles B. Geisler #248