

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 01/10/2017

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:20
INTERNAL STANDARD	VERIFIED	01:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:20
BLANK TEST	0.00	01:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:21
BLANK TEST	0.00	01:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:23
BLANK TEST	0.00	01:24

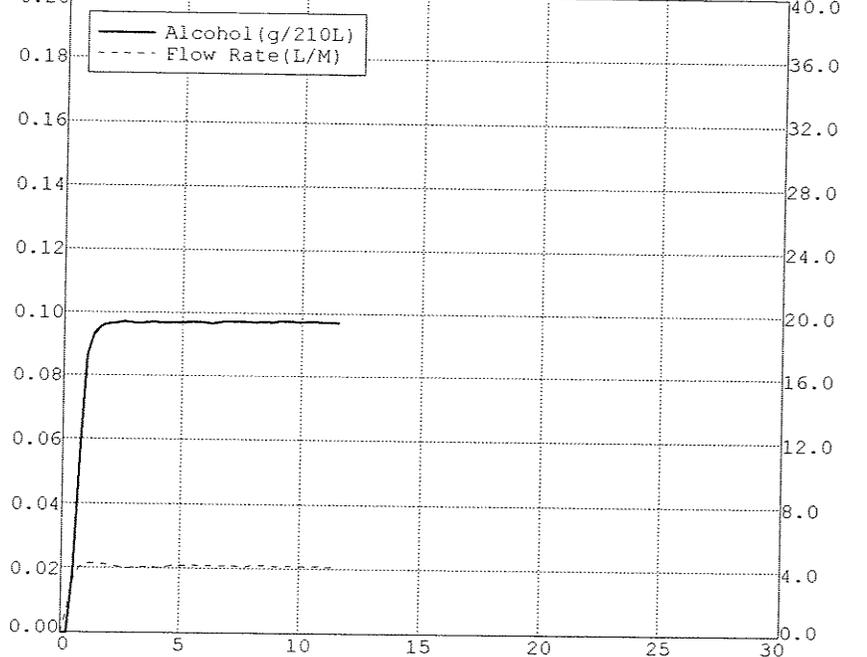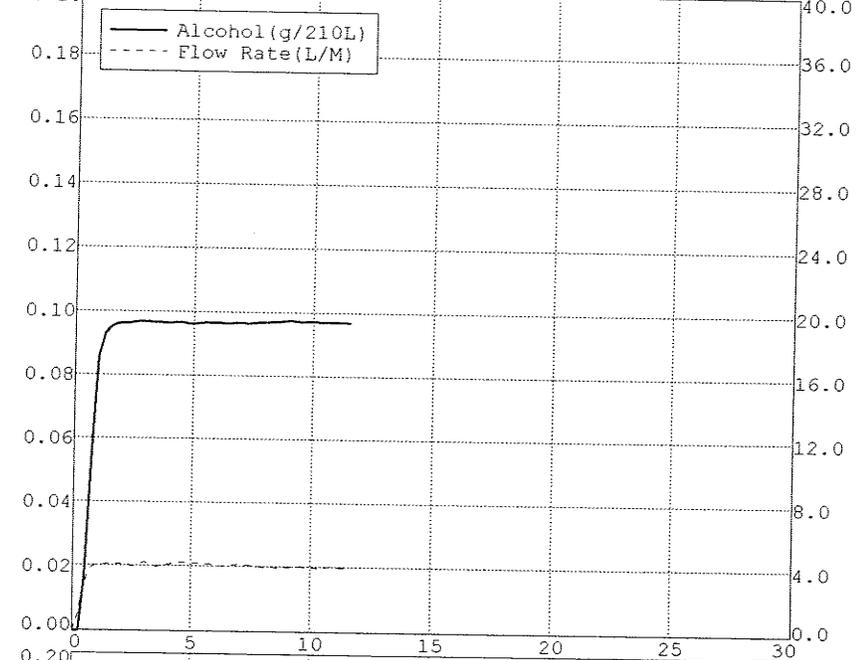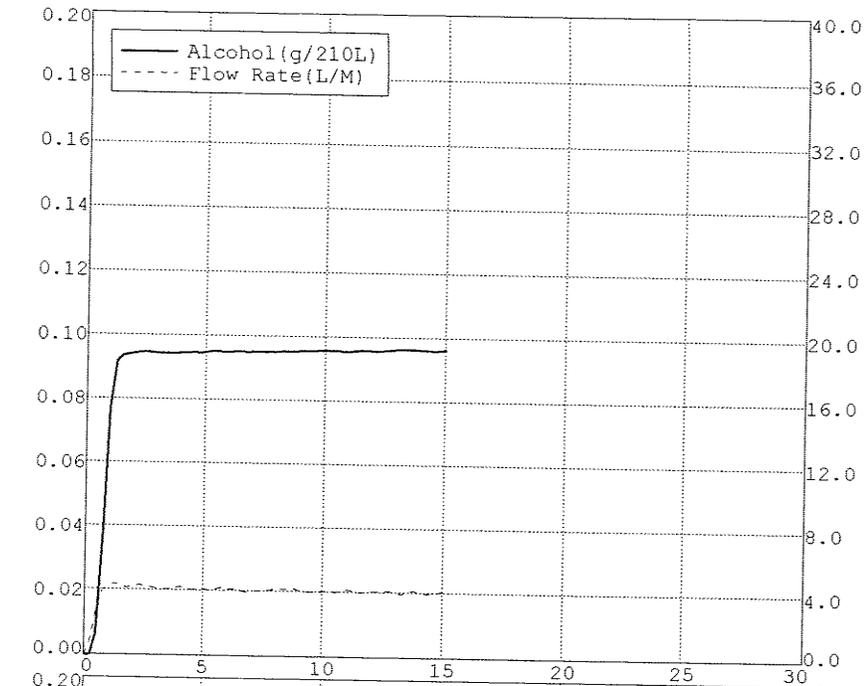

SUS BY / [Signature] WCSO #162
01-10-17