

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 01/16/2017

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16240

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:17
INTERNAL STANDARD	VERIFIED	01:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:18
BLANK TEST	0.00	01:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:19
BLANK TEST	0.00	01:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:21
BLANK TEST	0.00	01:22

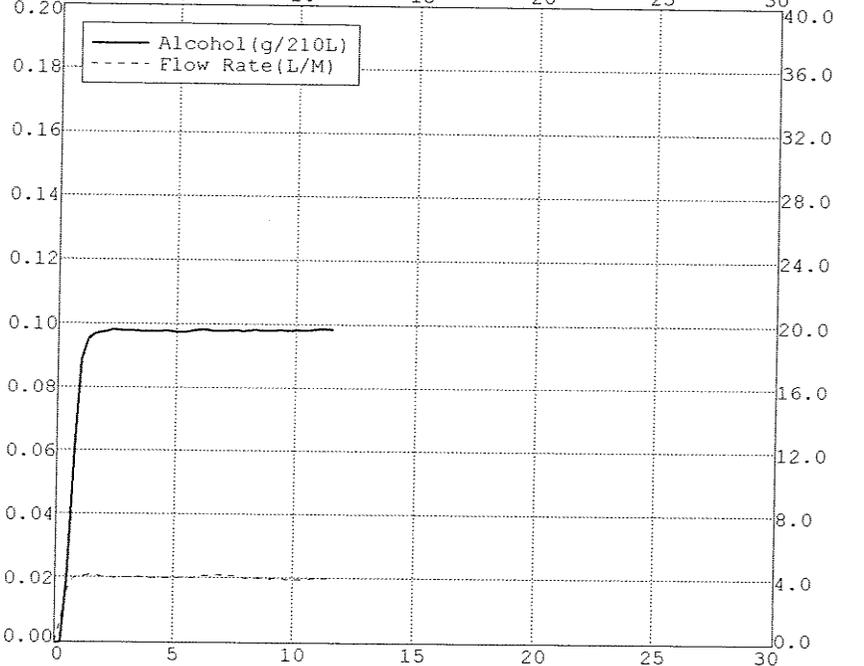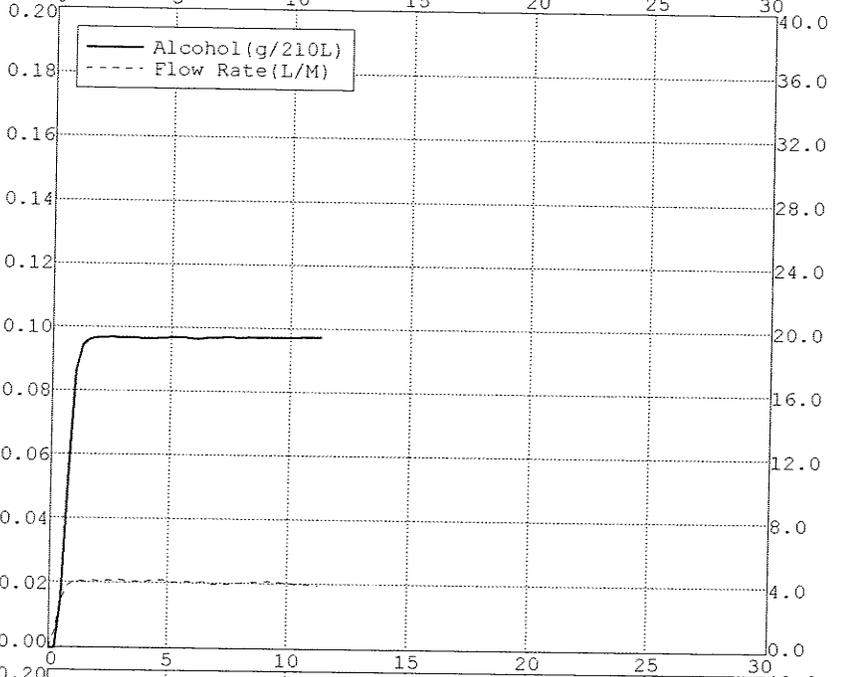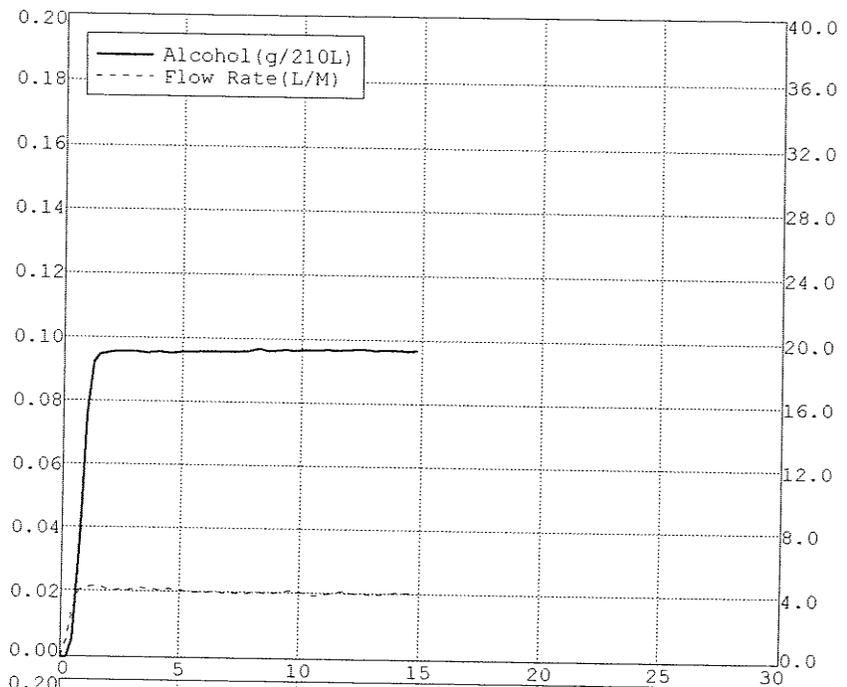

SGT Ralph J Bartlett WCSO #162
01-16-17