

SOLUTION CHANGE



WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/30/2017

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:56
INTERNAL STANDARD	VERIFIED	00:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:57
BLANK TEST	0.00	00:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:58
BLANK TEST	0.00	00:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:59
BLANK TEST	0.00	01:00

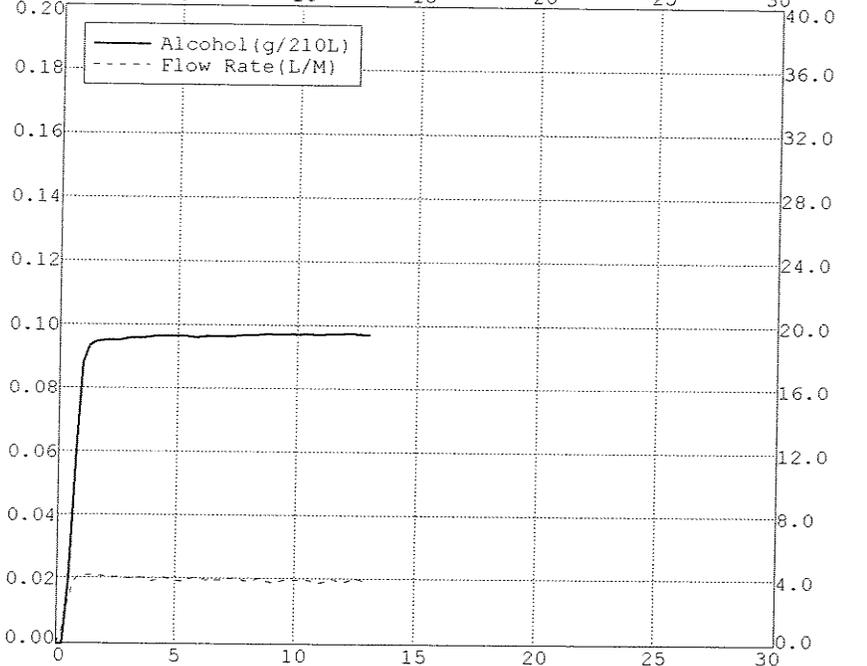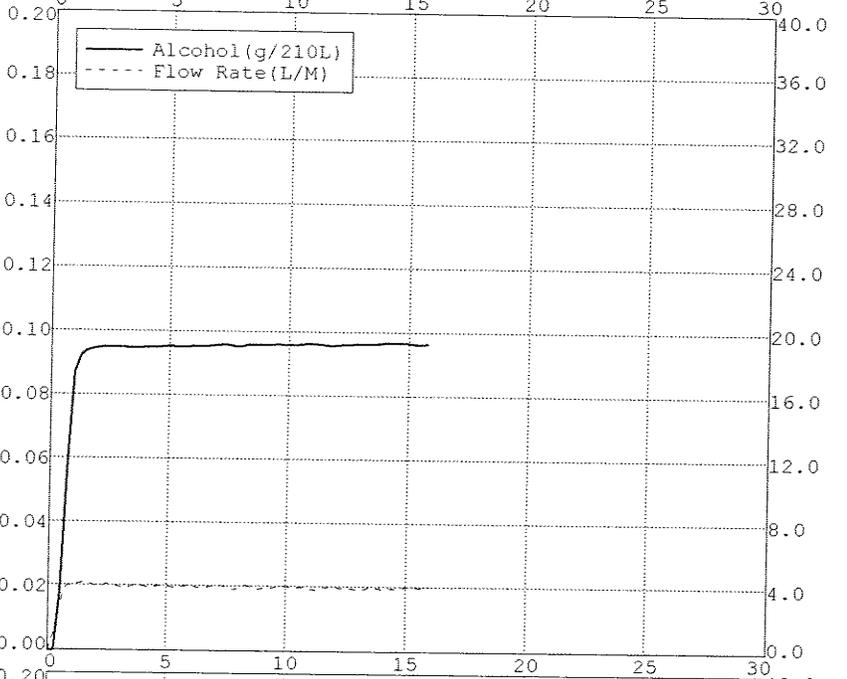

SES By *[Signature]* Shield # *[Signature]*  
01-30-17