

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 02/13/2017

OPERATOR NAME:  
 RALPH J BARTLETT  
 Permit #: 26222  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 16380

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 01:11 |
| INTERNAL STANDARD       | VERIFIED | 01:11 |
| REFERENCE STANDARD TEMP | 34.00c   |       |
| REFERENCE STANDARD      | 0.09     | 01:12 |
| BLANK TEST              | 0.00     | 01:13 |
| REFERENCE STANDARD TEMP | 34.02c   |       |
| REFERENCE STANDARD      | 0.09     | 01:13 |
| BLANK TEST              | 0.00     | 01:14 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.09     | 01:14 |
| BLANK TEST              | 0.00     | 01:15 |

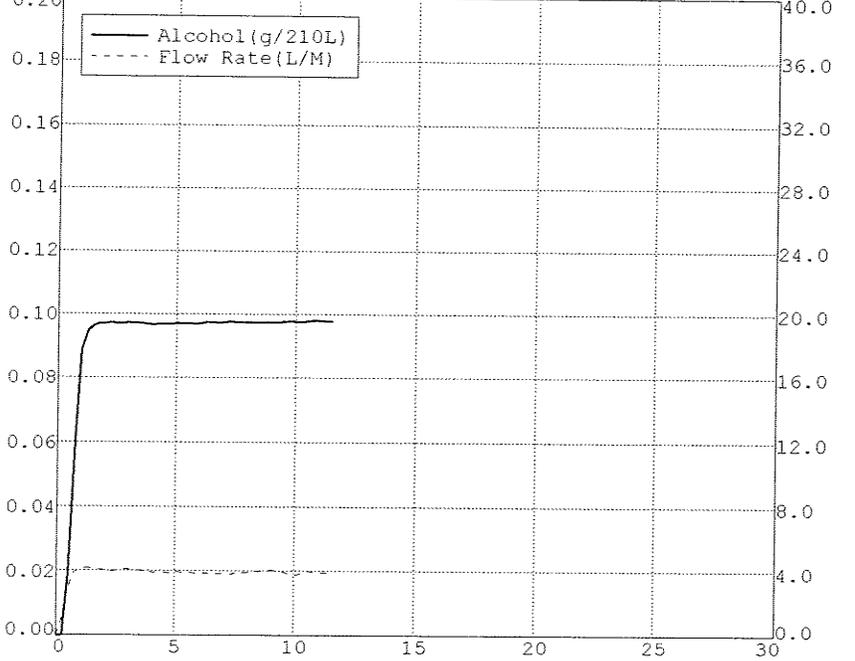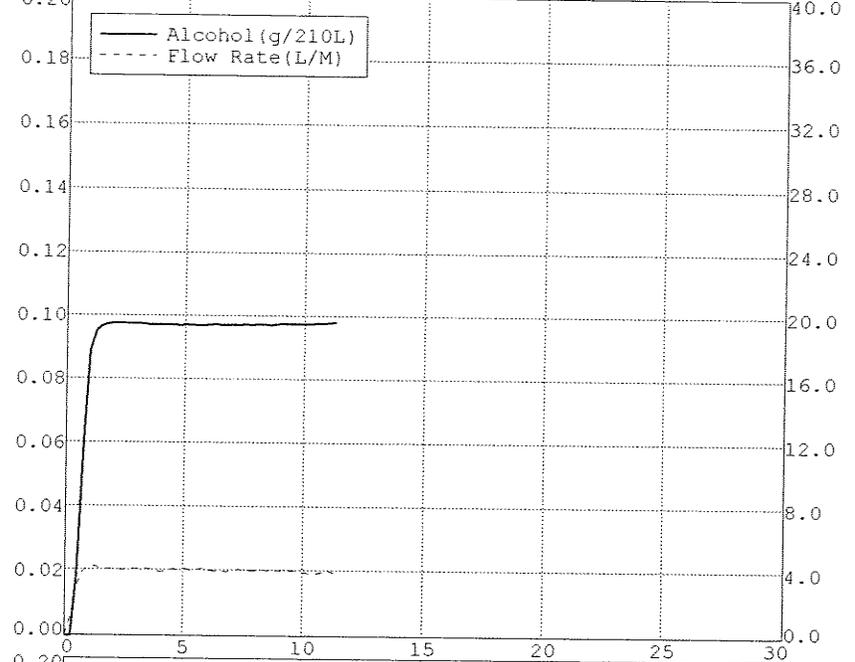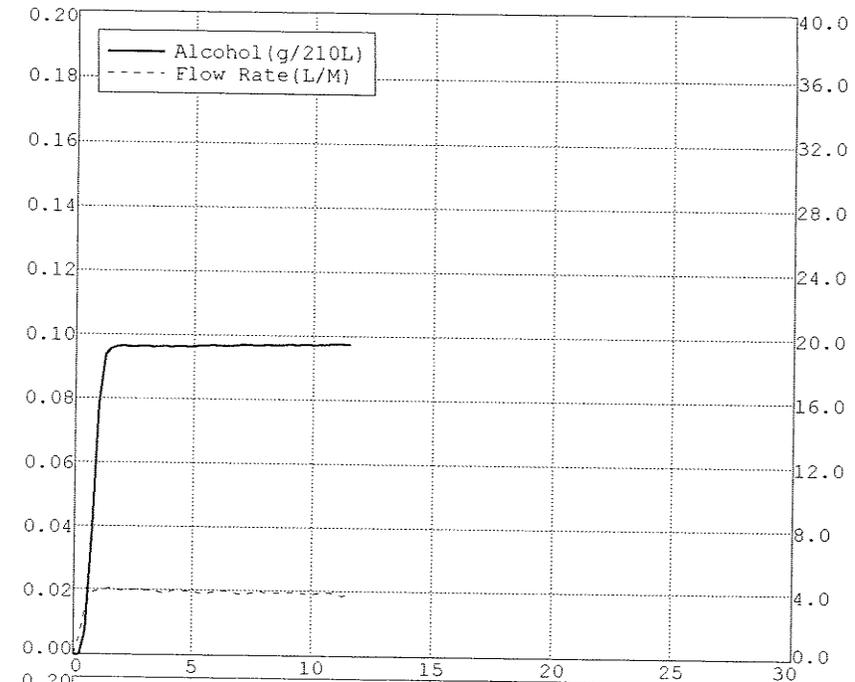

SG *Ralph Bartlett* WCSO #162  
 02-13-17