

SUPERVISOR TEST



WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/27/2017

OPERATOR NAME:  
RALPH J BARTLETT  
Permit #: 26222  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:03
INTERNAL STANDARD	VERIFIED	00:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:03
BLANK TEST	0.00	00:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:05
BLANK TEST	0.00	00:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:06
BLANK TEST	0.00	00:07

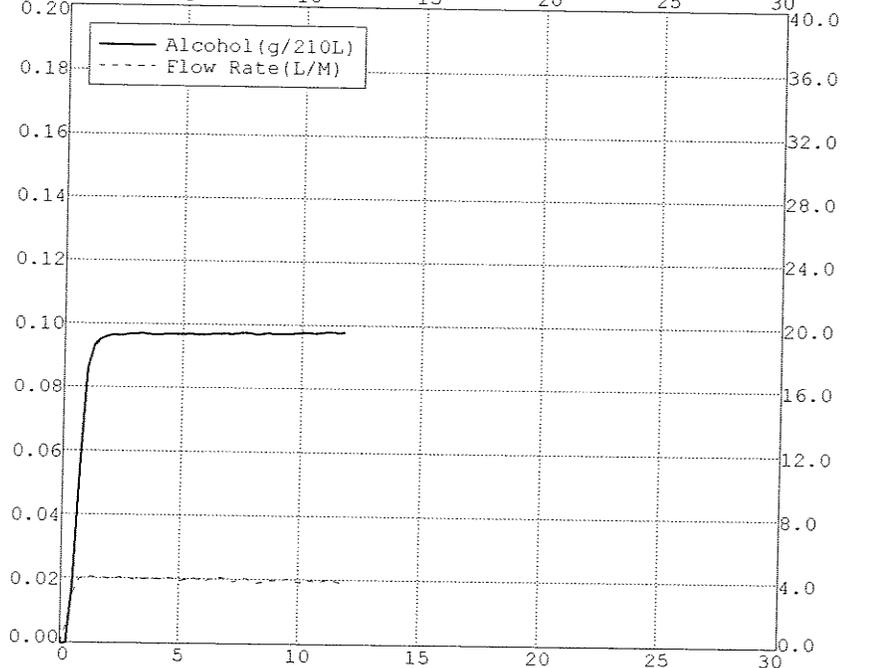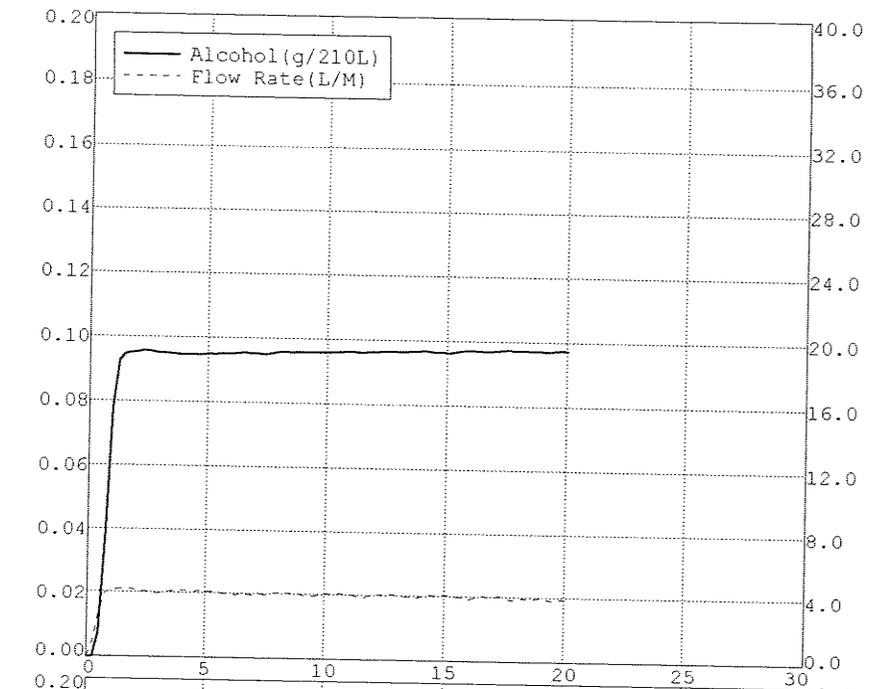

SG: RJB / JWB 2/27/17  
WCSO#162