

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/15/2017

OPERATOR NAME:
RALPH J BARTLETT
Permit #: 26222
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 16380

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:51
INTERNAL STANDARD	VERIFIED	22:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:52
BLANK TEST	0.00	22:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:53
BLANK TEST	0.00	22:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:54
BLANK TEST	0.00	22:55

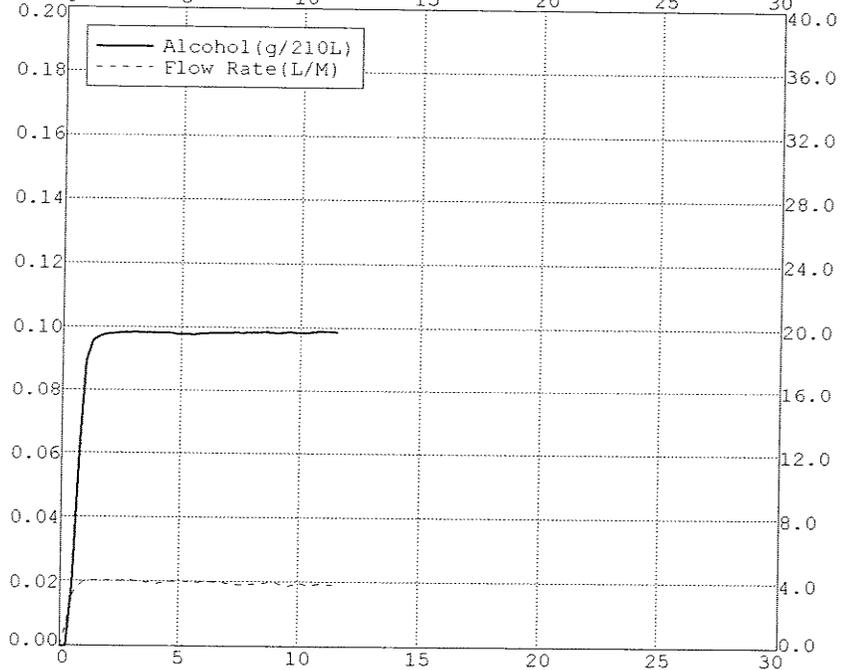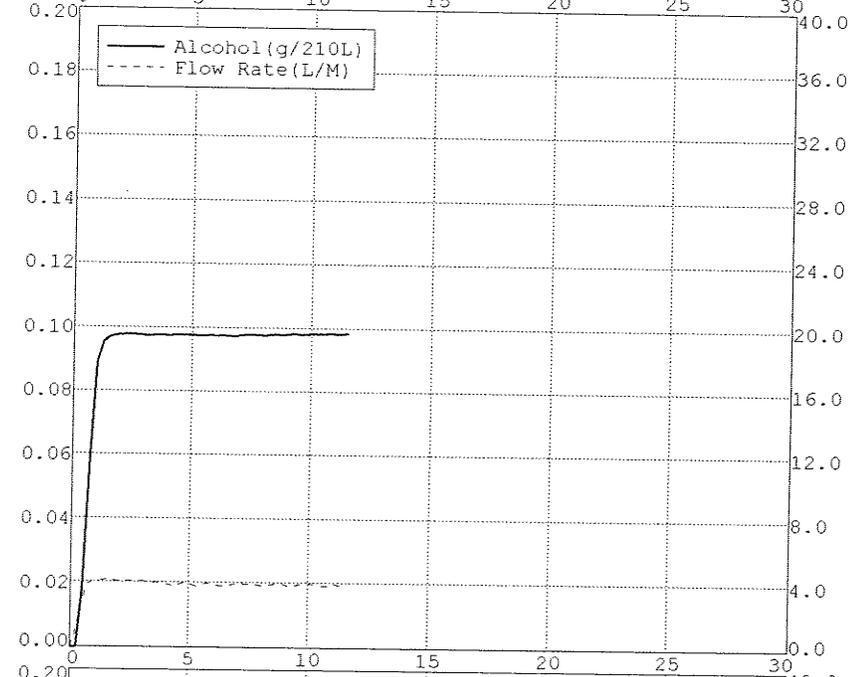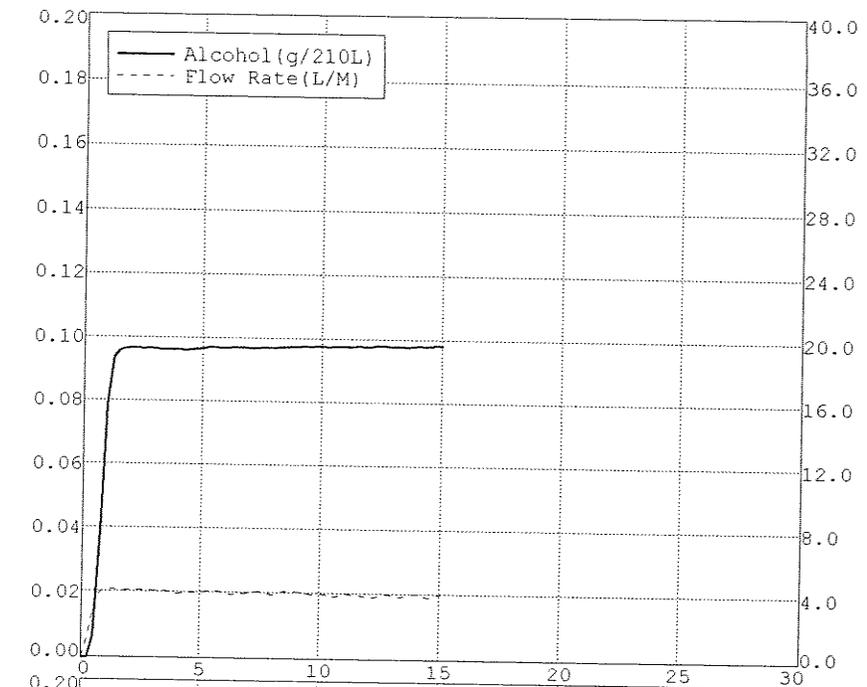

SCS RJB Bartlett WRSO #162
03-15-17