

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/22/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:58
INTERNAL STANDARD	VERIFIED	05:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	05:58
BLANK TEST	0.00	05:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:00
BLANK TEST	0.00	06:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	06:01
BLANK TEST	0.00	06:02

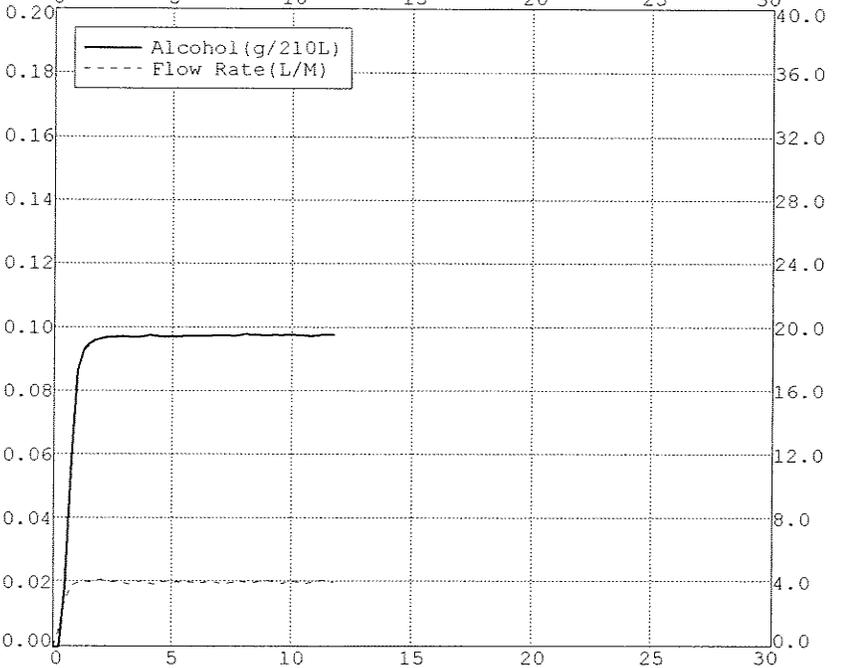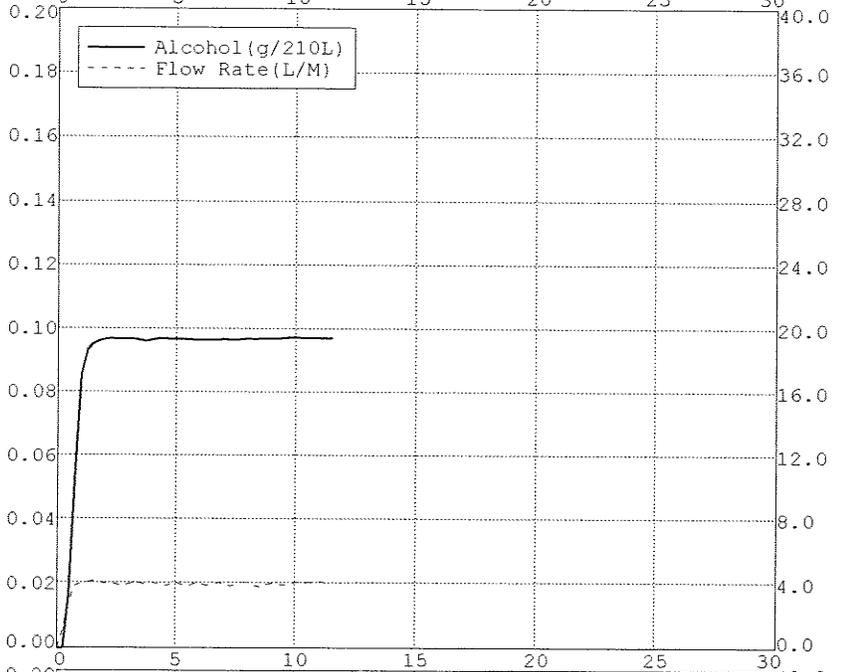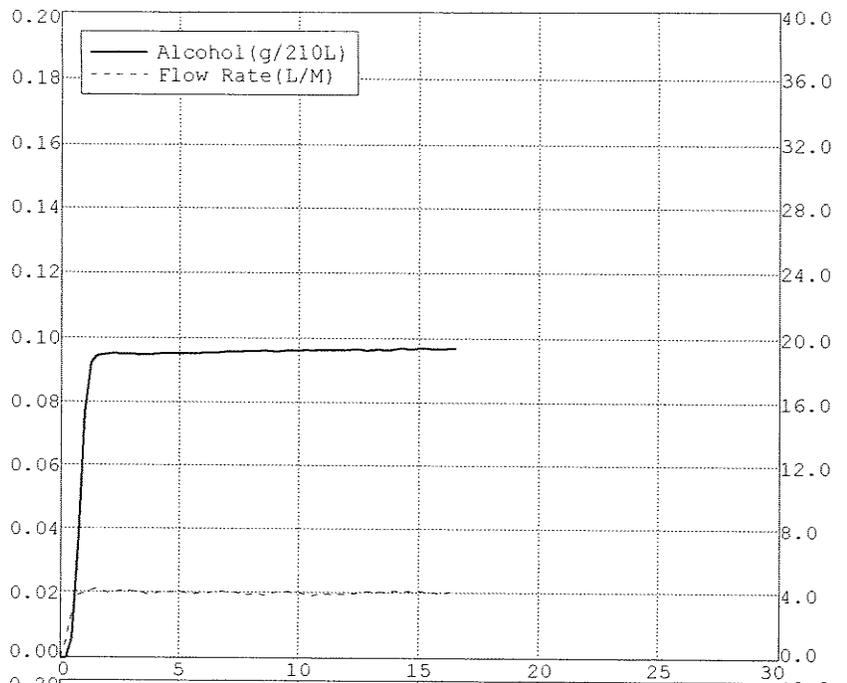

See also #248