

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/28/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:36
INTERNAL STANDARD	VERIFIED	00:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:37
BLANK TEST	0.00	00:38
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:38
BLANK TEST	0.00	00:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:39
BLANK TEST	0.00	00:40

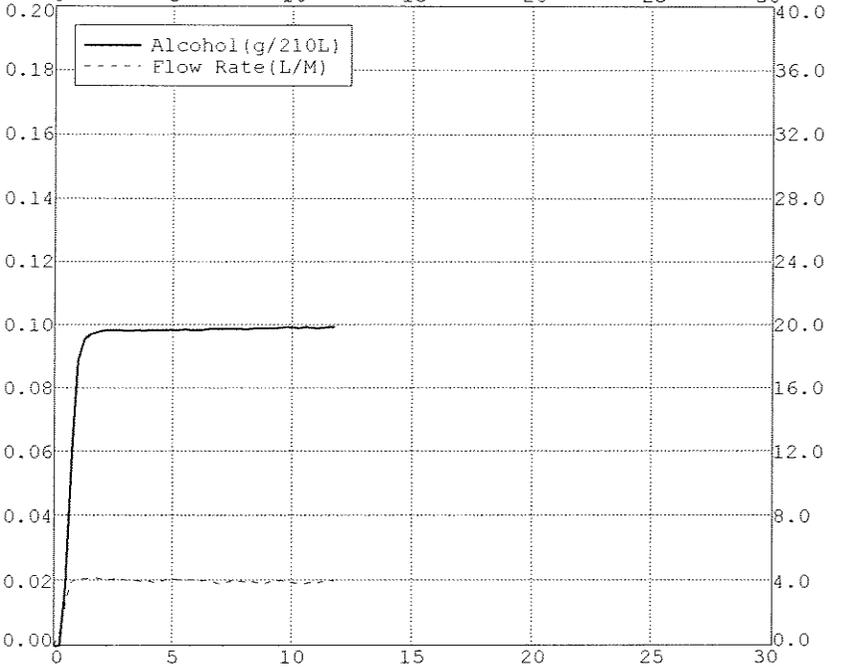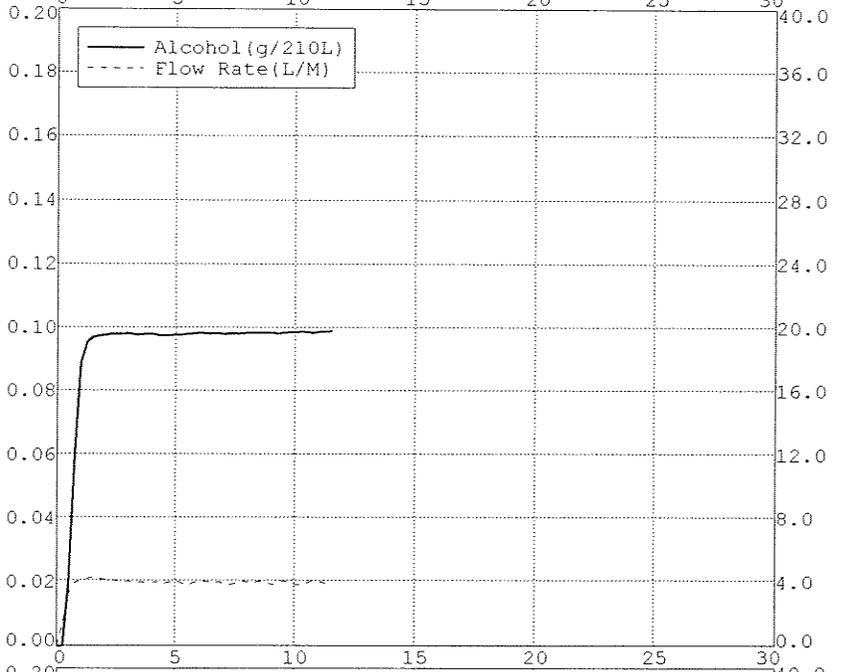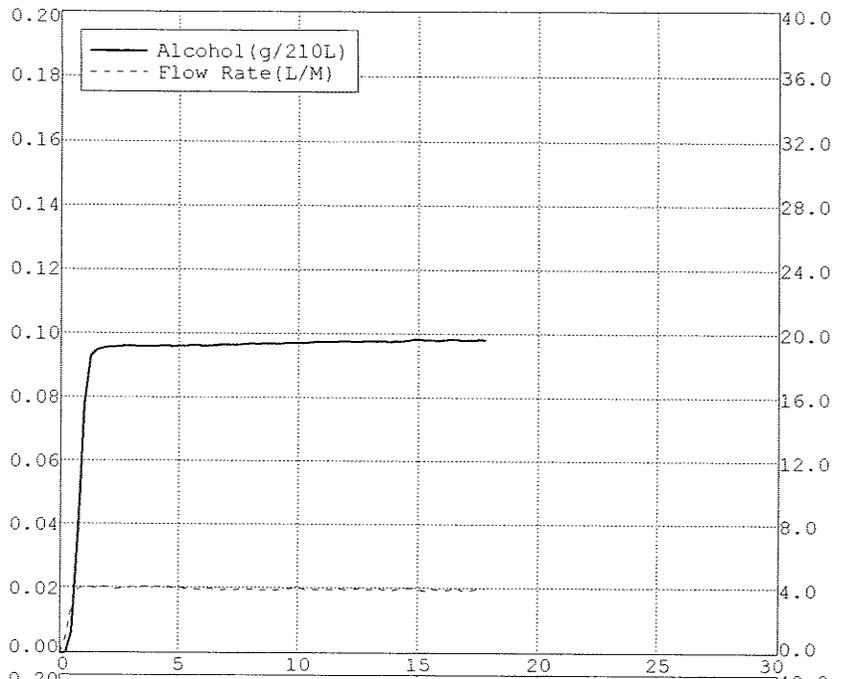

Charles B. Geisler
4/28/17