

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/02/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:34
INTERNAL STANDARD	VERIFIED	03:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:34
BLANK TEST	0.00	03:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:35
BLANK TEST	0.00	03:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:37
BLANK TEST	0.00	03:38

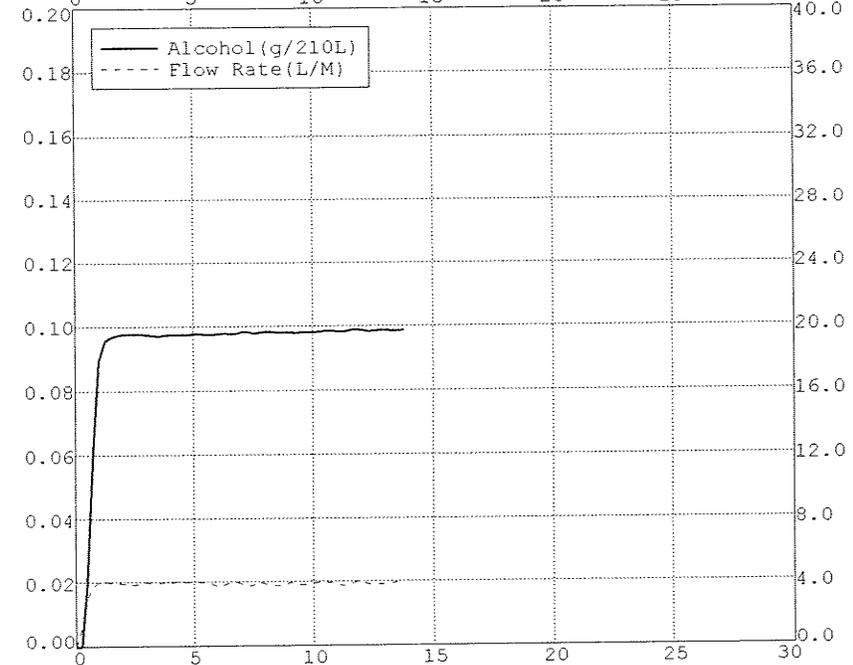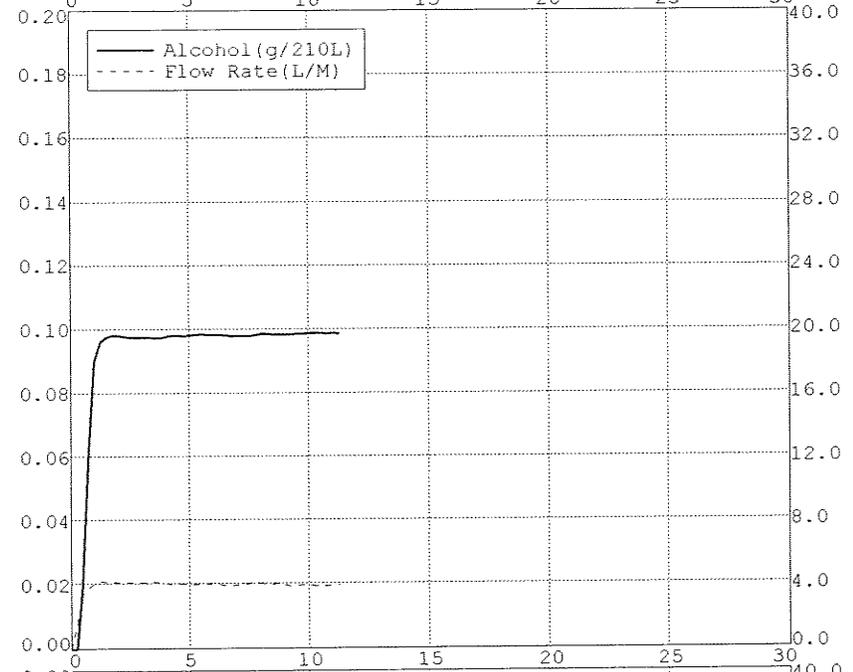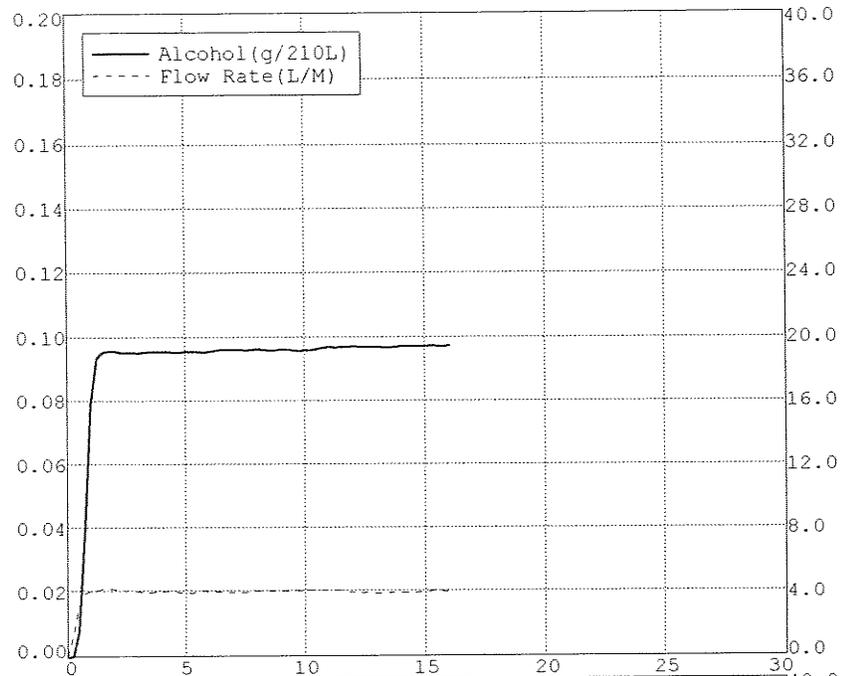

Charles B. Geisler #245