

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/11/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:17
INTERNAL STANDARD	VERIFIED	01:17
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	01:18
BLANK TEST	0.00	01:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:19
BLANK TEST	0.00	01:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:20
BLANK TEST	0.00	01:21

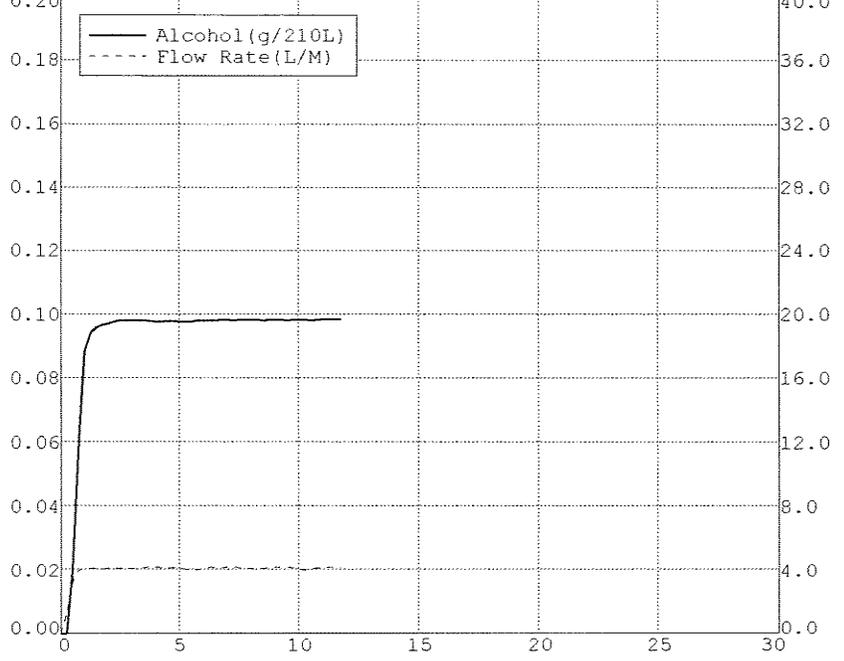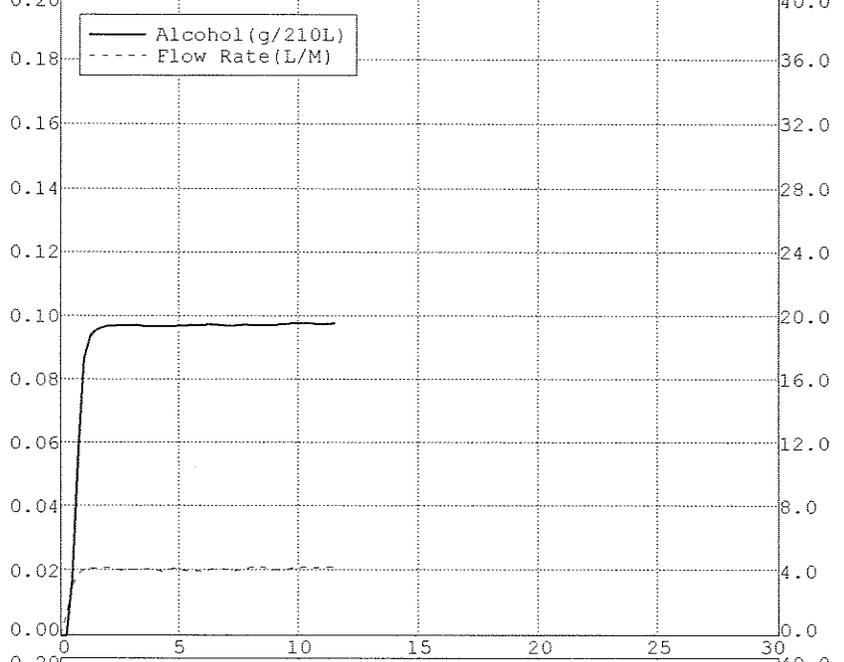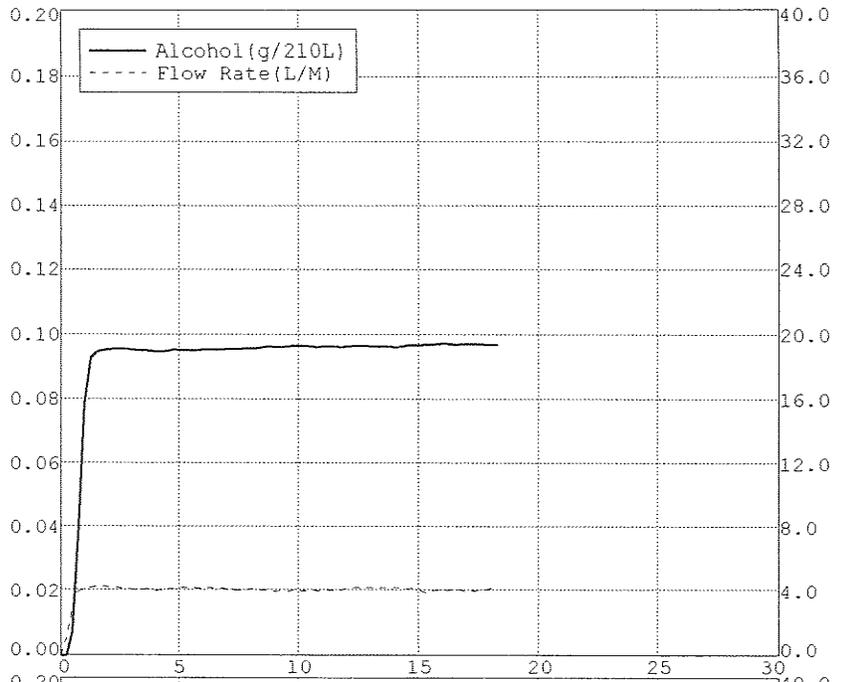

Charles B Geisler #204