

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 05/15/2017

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:17
INTERNAL STANDARD	VERIFIED	10:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:17
BLANK TEST	0.00	10:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:19
BLANK TEST	0.00	10:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:20
BLANK TEST	0.00	10:21

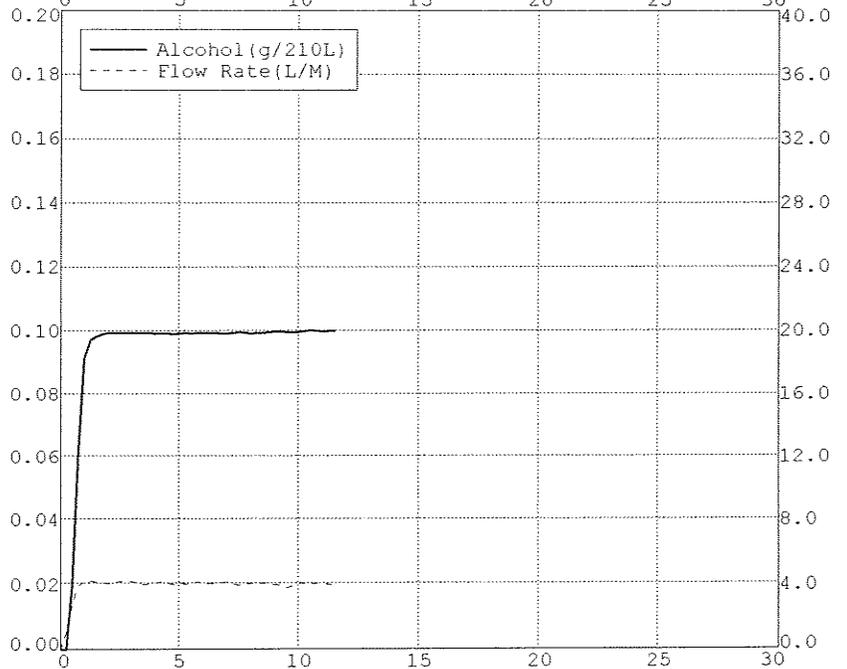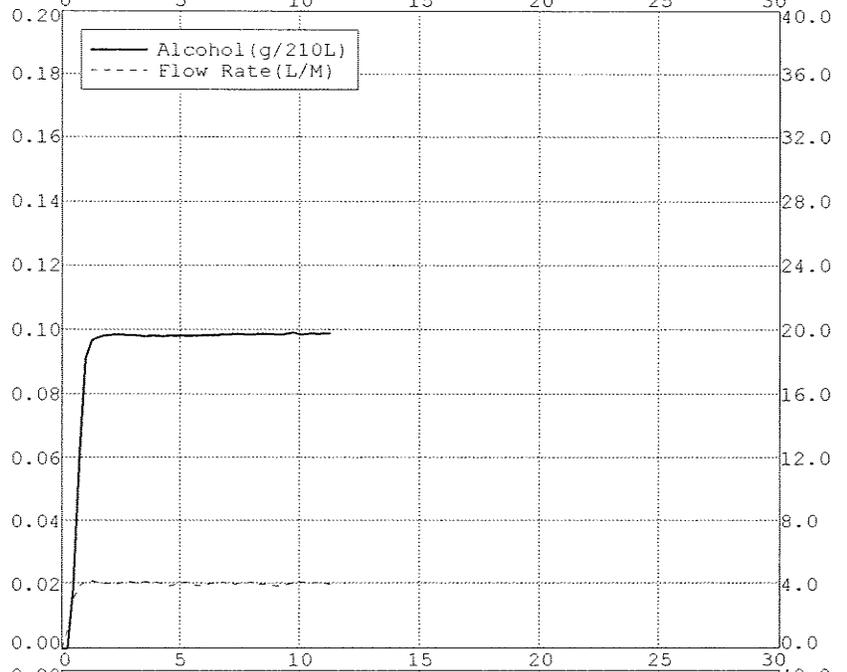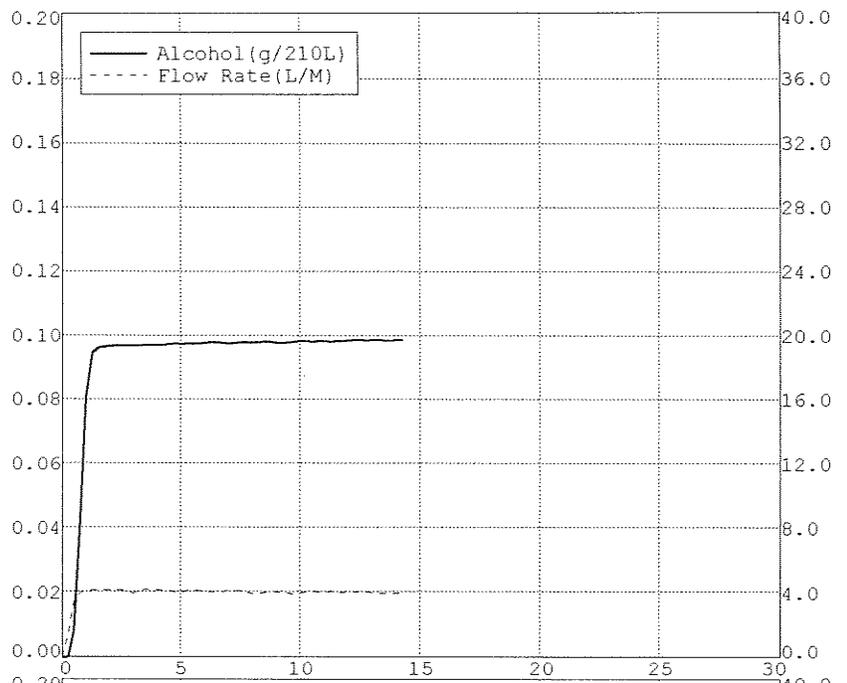

Charles B. Geisler 5/15/17