

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 05/29/2017

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:00
INTERNAL STANDARD	VERIFIED	00:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:01
BLANK TEST	0.00	00:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:02
BLANK TEST	0.00	00:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:03
BLANK TEST	0.00	00:04

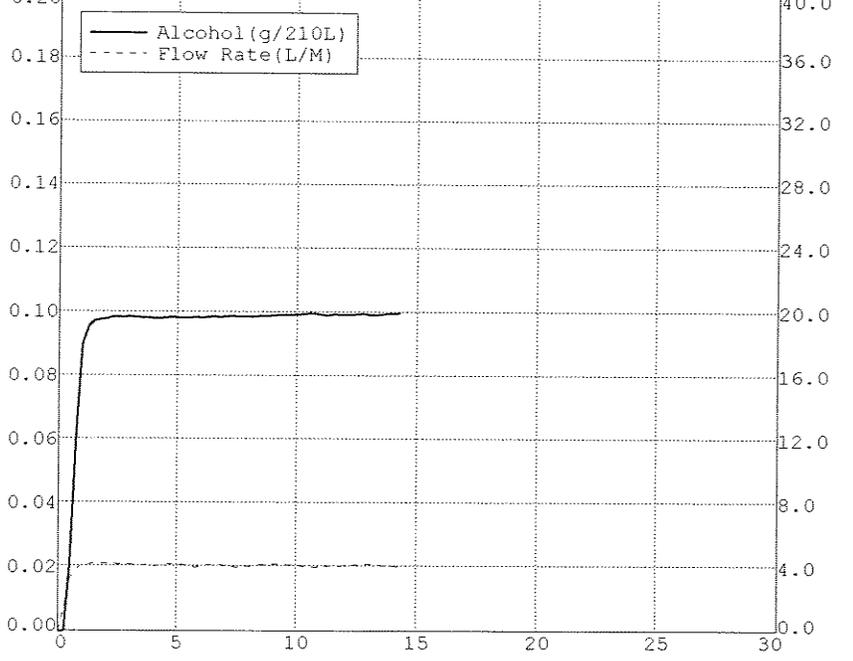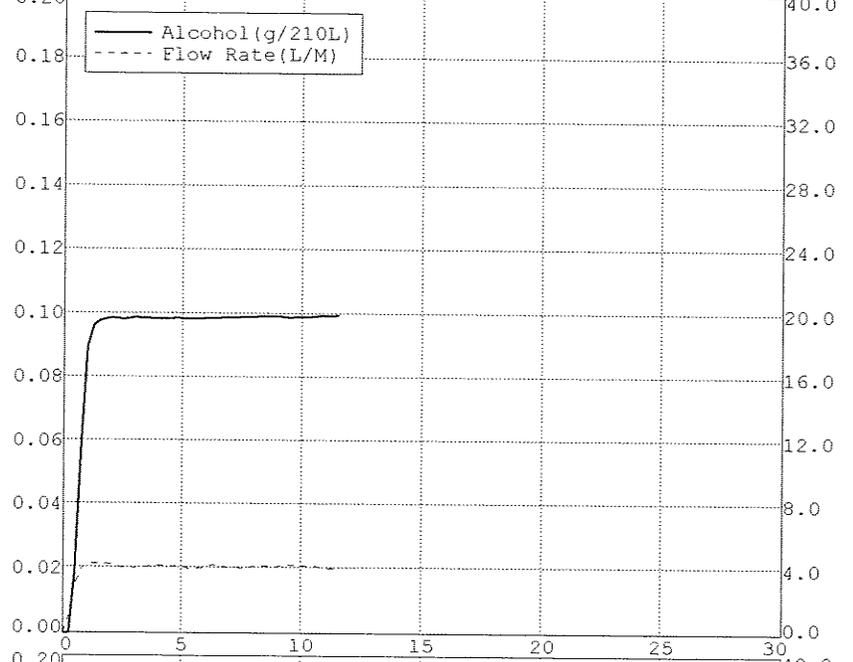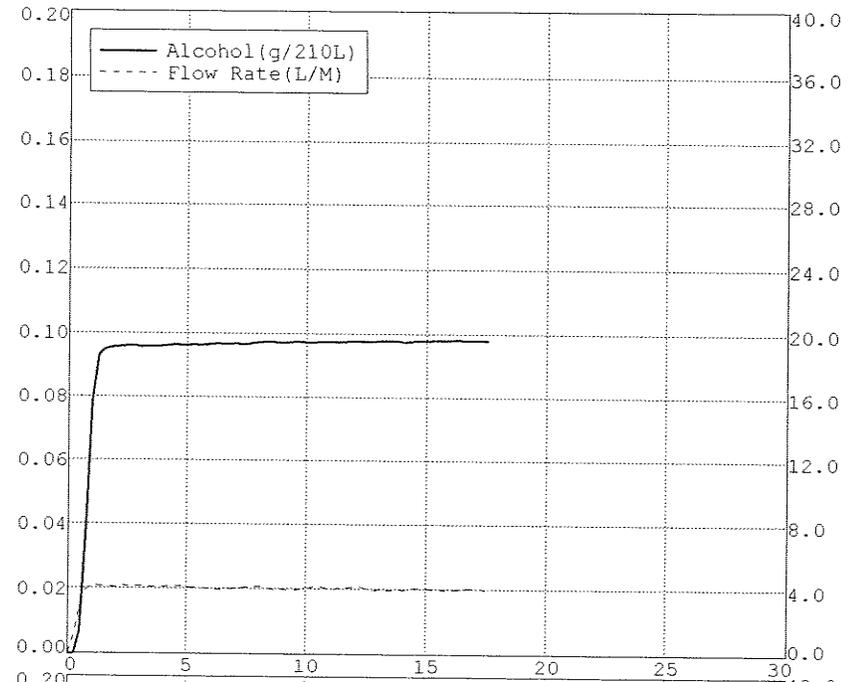

Charles B Geisler #245