

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 06/17/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:29
INTERNAL STANDARD	VERIFIED	03:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:30
BLANK TEST	0.00	03:31
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	03:31
BLANK TEST	0.00	03:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:32
BLANK TEST	0.00	03:33

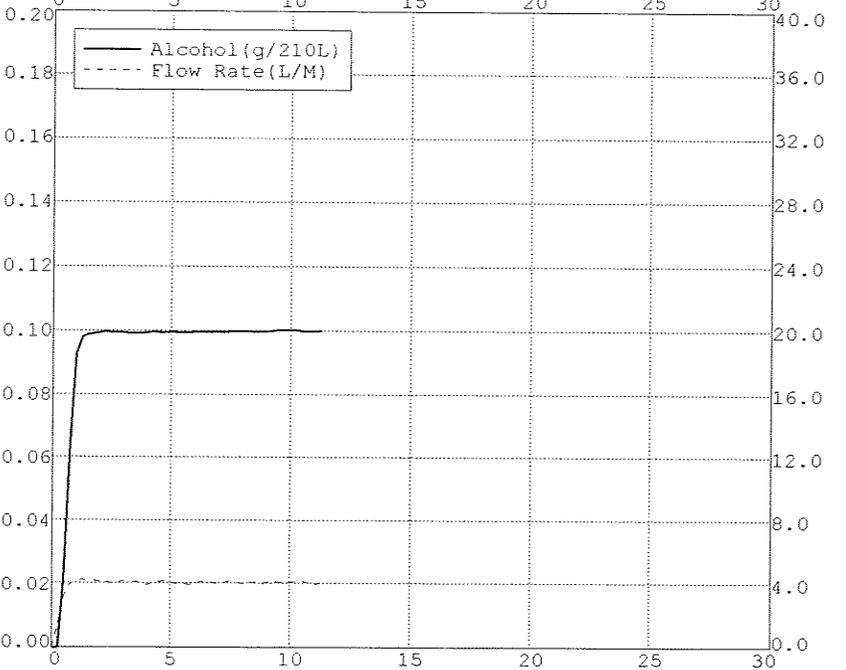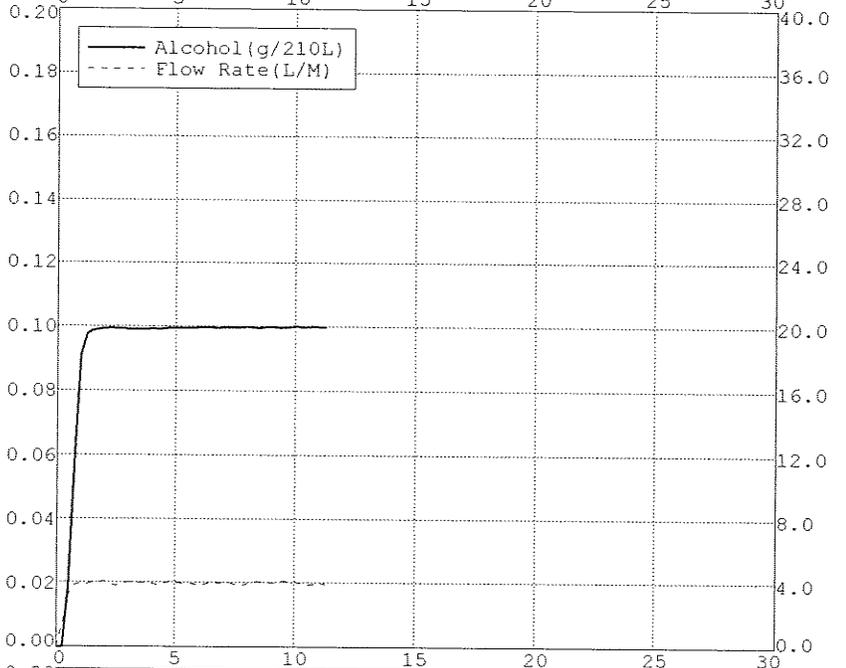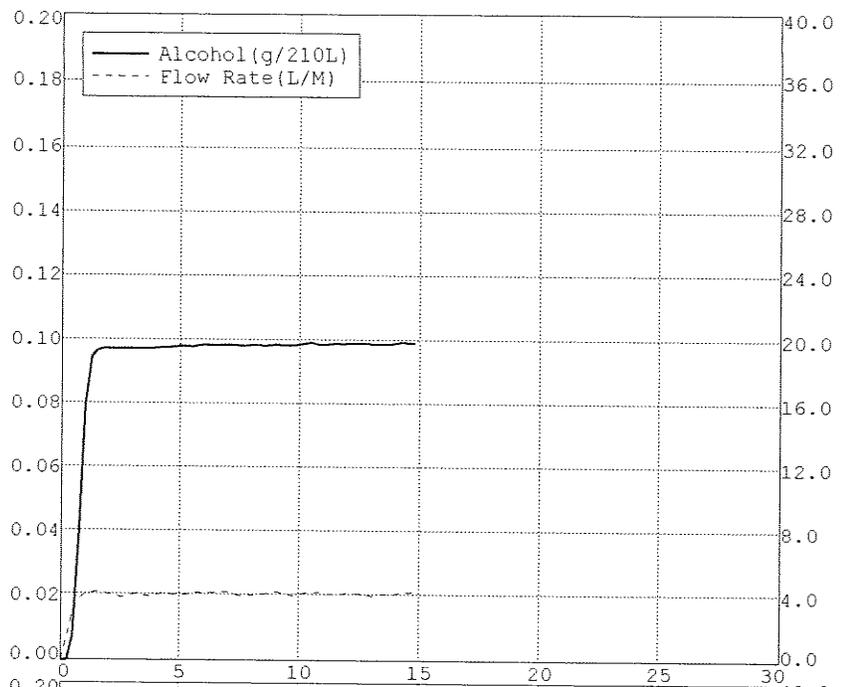

*Spec. Chd. B. [Signature] #241*