

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/01/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:23
INTERNAL STANDARD	VERIFIED	23:24
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	23:24
BLANK TEST	0.00	23:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:25
BLANK TEST	0.00	23:26
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:27
BLANK TEST	0.00	23:28

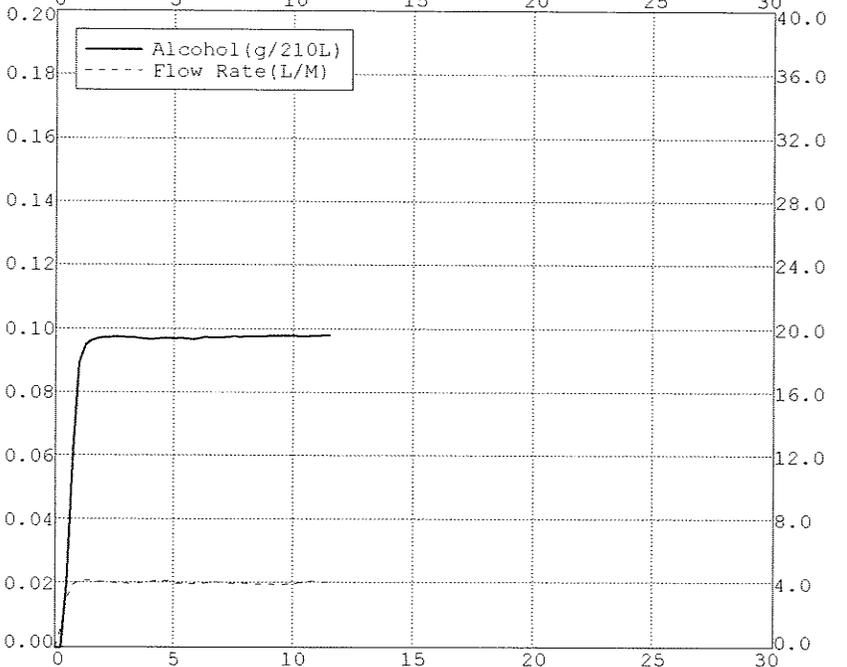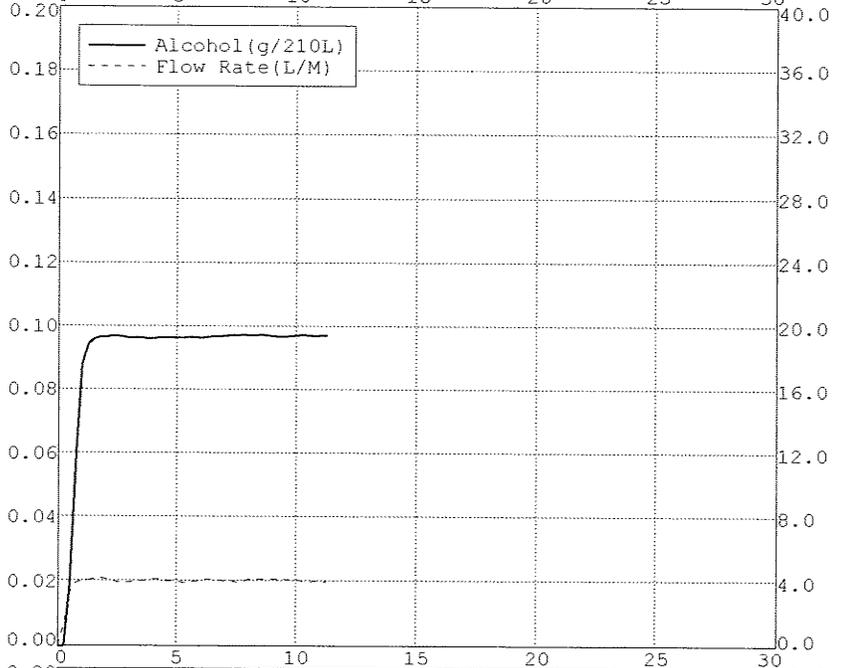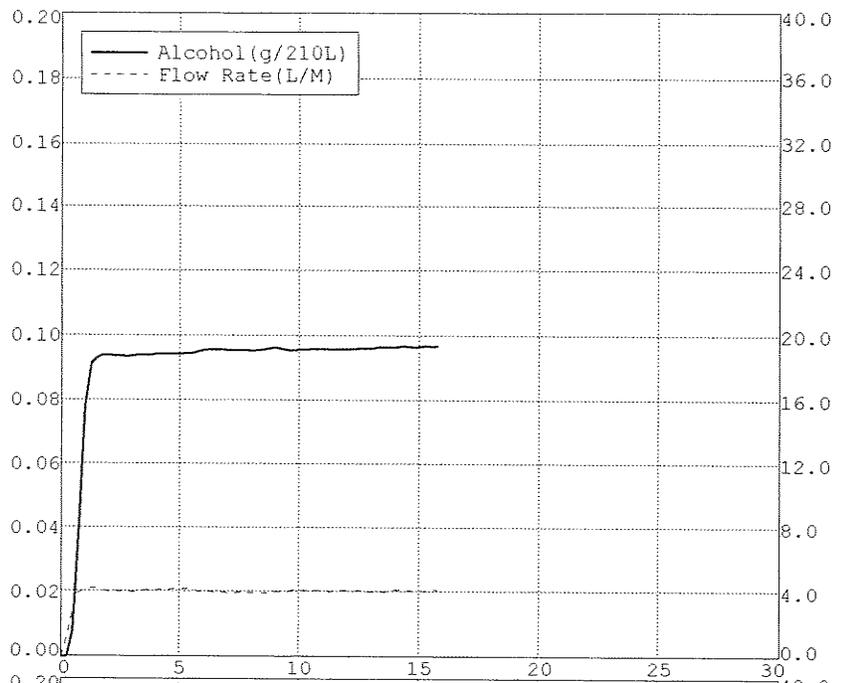

Sp. M. L. O'S #2018