

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 07/10/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:40
INTERNAL STANDARD	VERIFIED	23:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:40
BLANK TEST	0.00	23:41
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:41
BLANK TEST	0.00	23:42
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:43
BLANK TEST	0.00	23:44

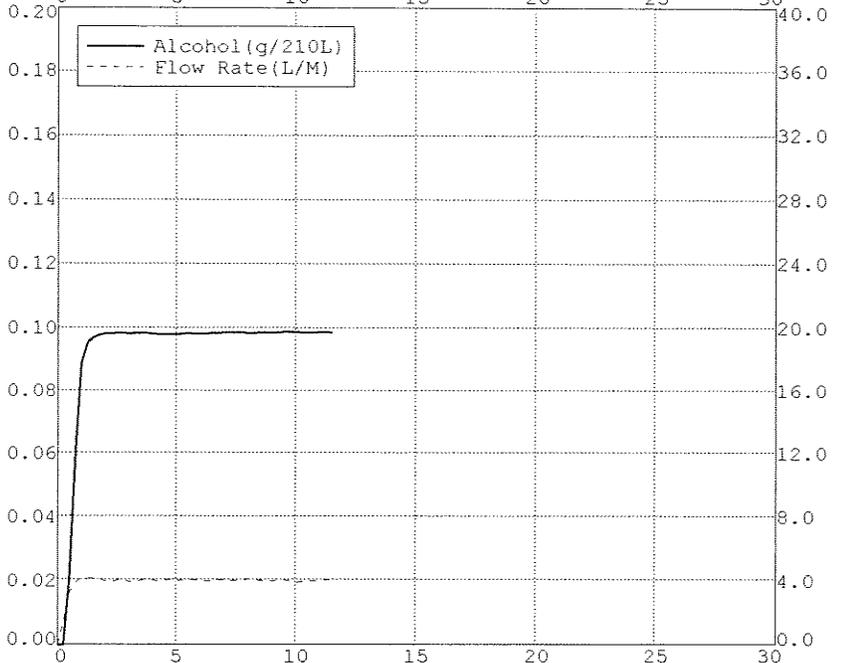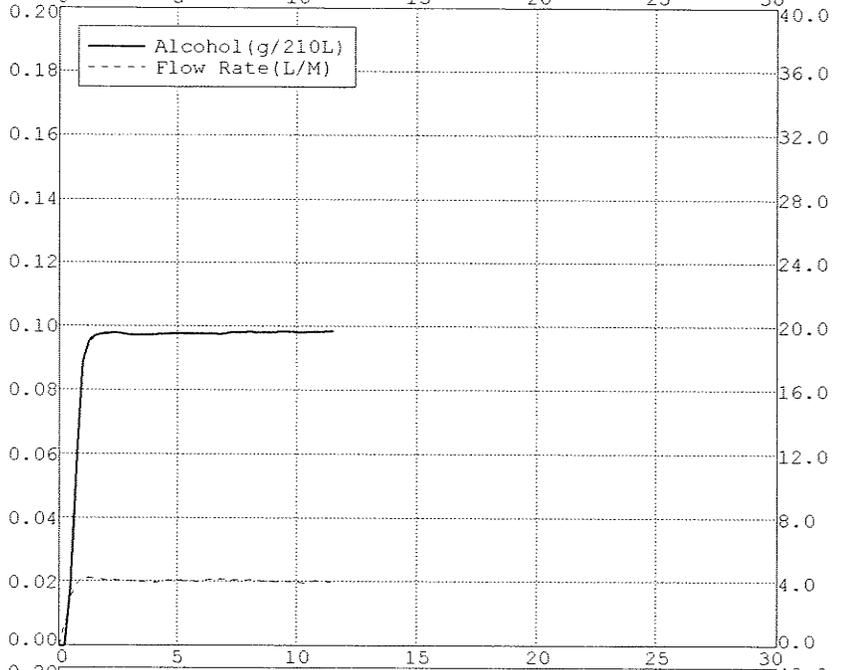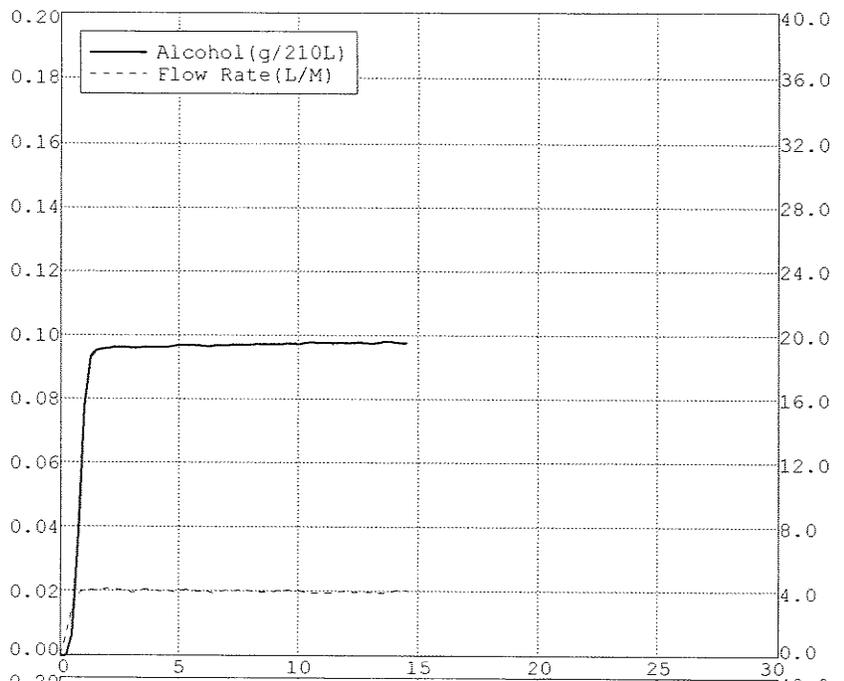

*Charles B. Geisler #295*