

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 07/11/2017

OPERATOR NAME:  
TYLER J MORSE  
Permit #: 41959  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:00
INTERNAL STANDARD	VERIFIED	18:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:01
BLANK TEST	0.00	18:02
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:02
BLANK TEST	0.00	18:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:03
BLANK TEST	0.00	18:04

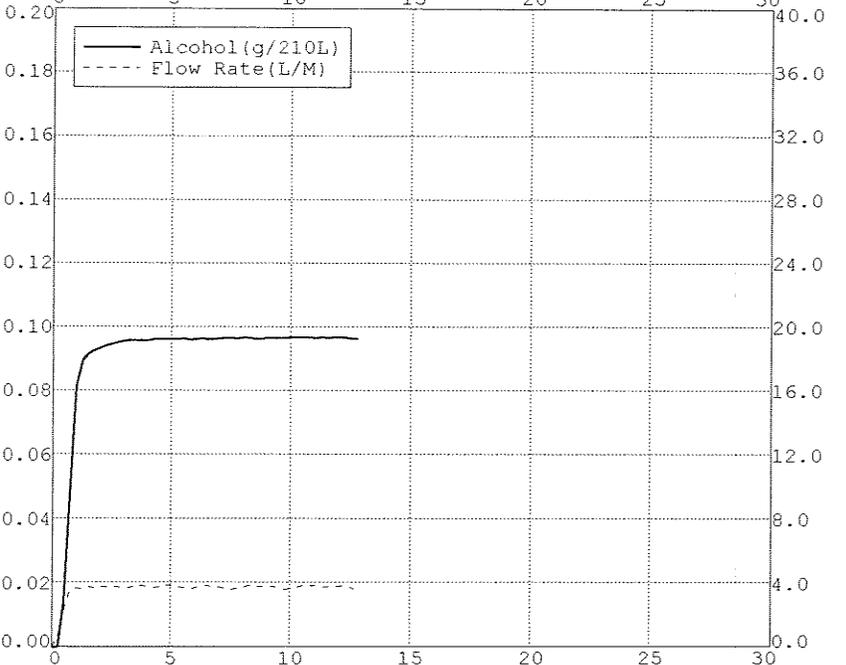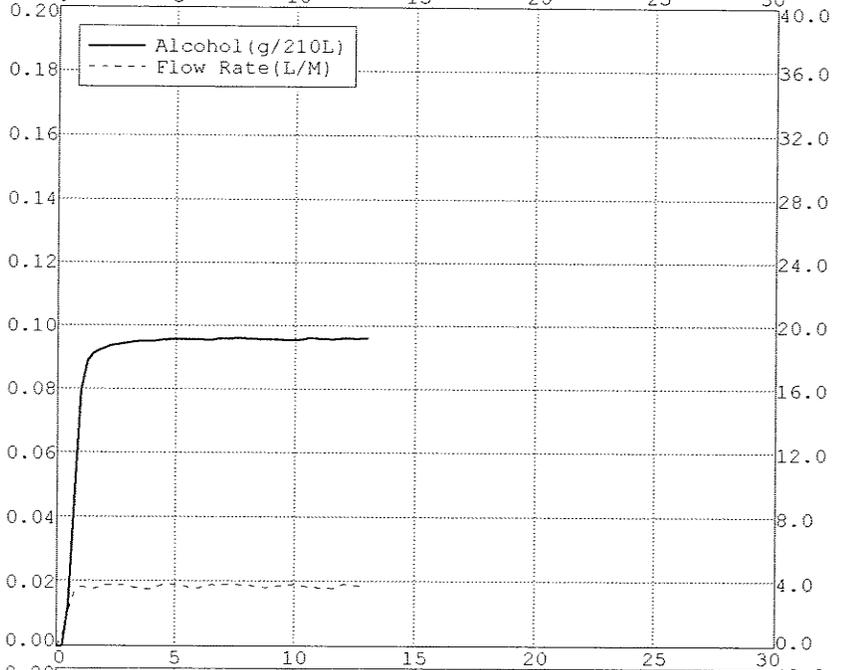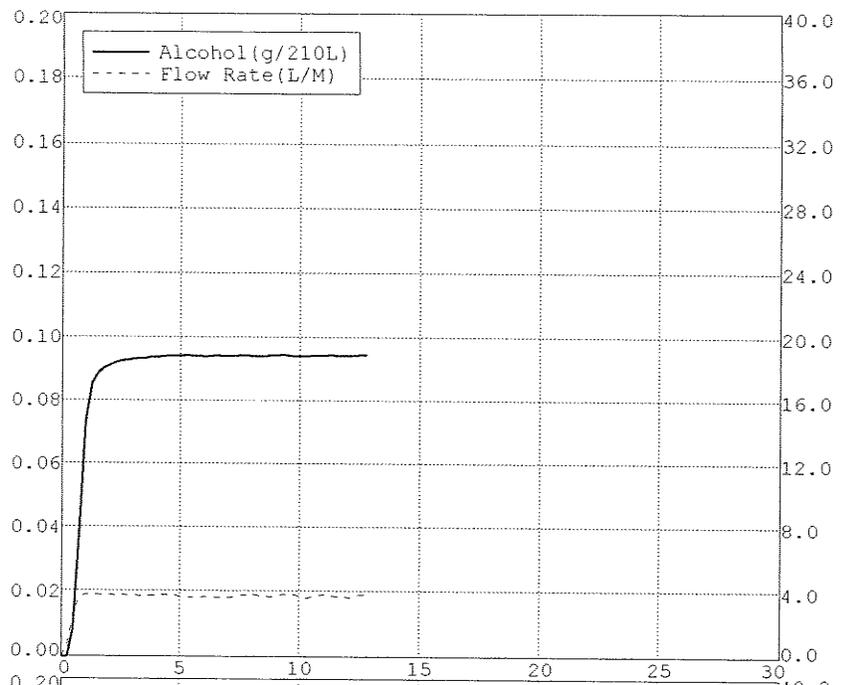

*Ps L2 #147*

SOLUTION CHANGE

-----  
WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208  
-----


Date: 07/11/2017

OPERATOR NAME:  
TYLER J MORSE  
Permit #: 41959  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:38
INTERNAL STANDARD	VERIFIED	17:38
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.08	17:38

Blank Error

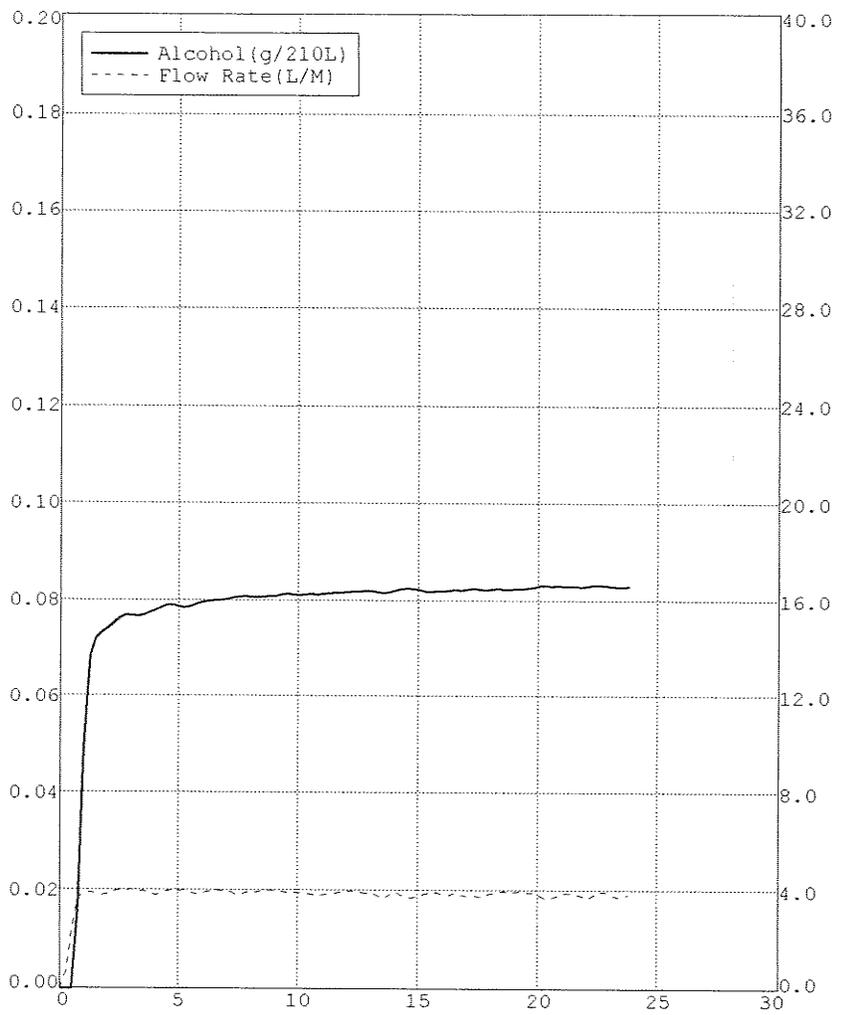

*(Signature) #447*

SOLUTION CHANGE

-----  
WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208  
-----


Date: 07/11/2017

OPERATOR NAME:  
TYLER J MORSE  
Permit #: 41959  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:54
INTERNAL STANDARD	VERIFIED	17:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:54

Blank Error

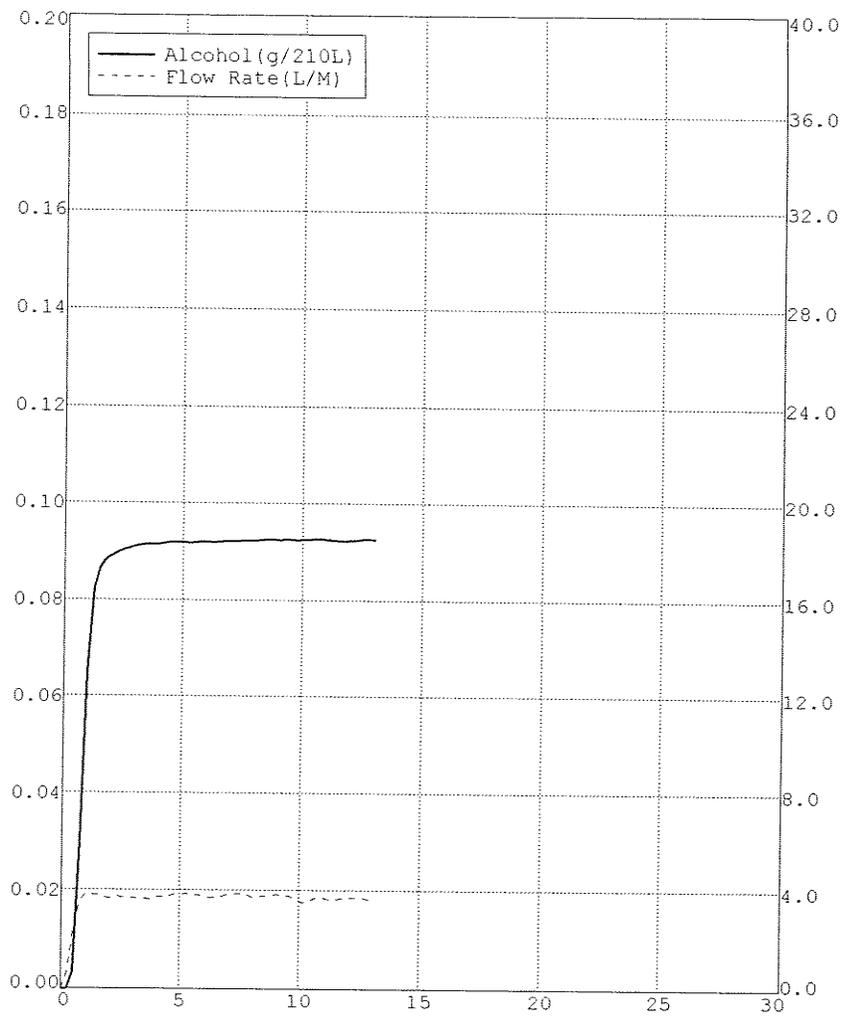

PL #447