

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 07/17/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:44
INTERNAL STANDARD	VERIFIED	00:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:44
BLANK TEST	0.00	00:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:45
BLANK TEST	0.00	00:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:47
BLANK TEST	0.00	00:48

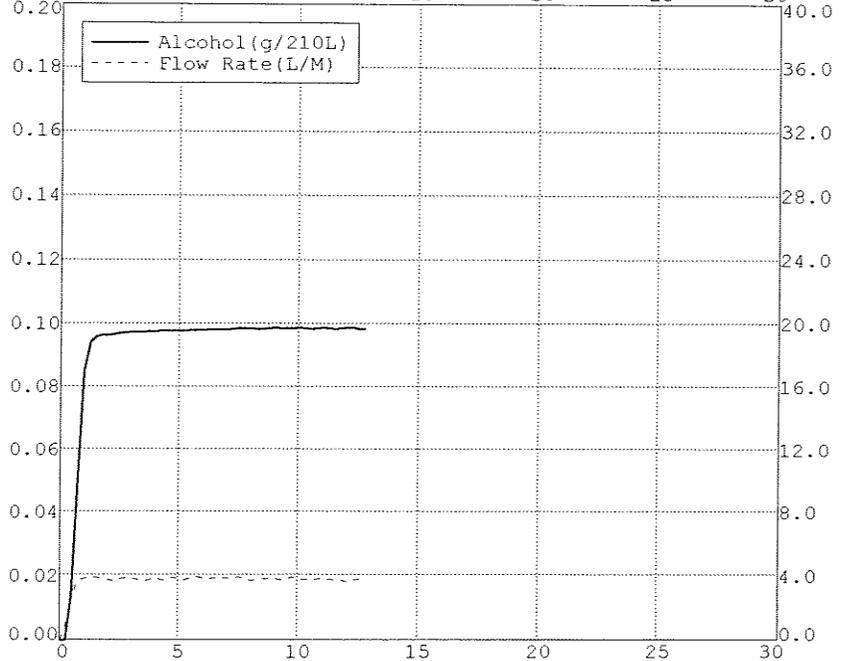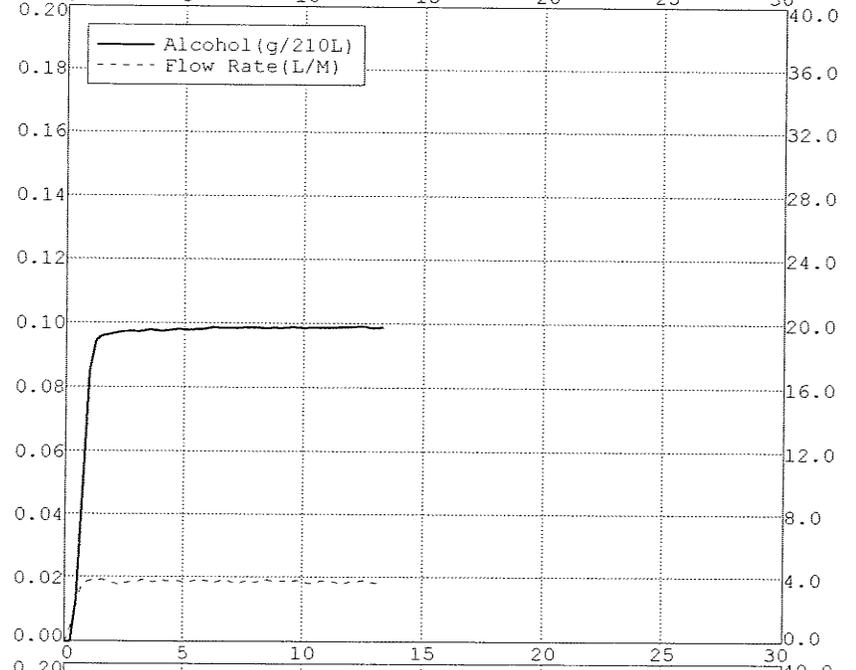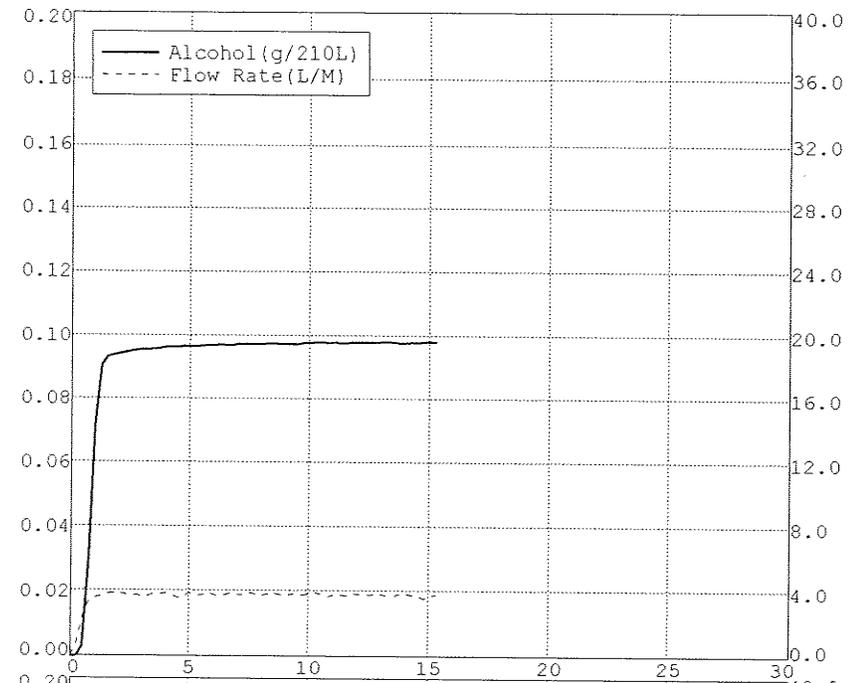

*Charles B. Geisler #296*